

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 01/13/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:36
INTERNAL STANDARD	VERIFIED	02:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:36
BLANK TEST	0.00	02:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	02:37
BLANK TEST	0.00	02:38
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	02:38
BLANK TEST	0.00	02:39

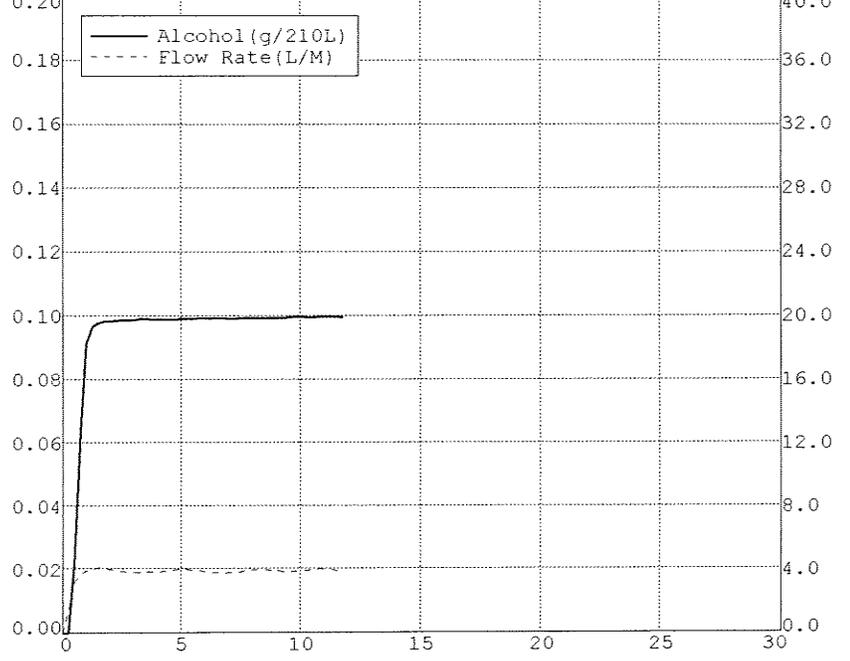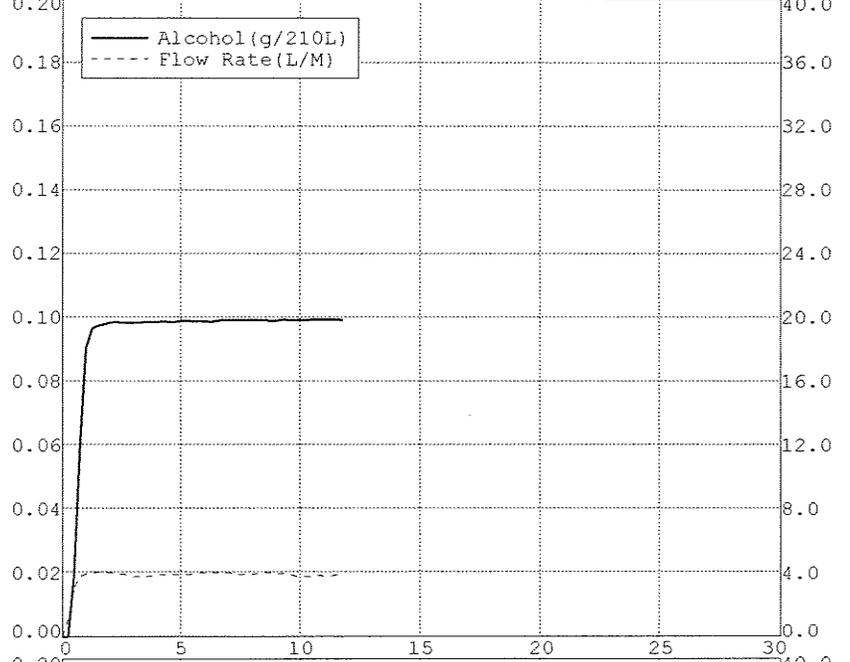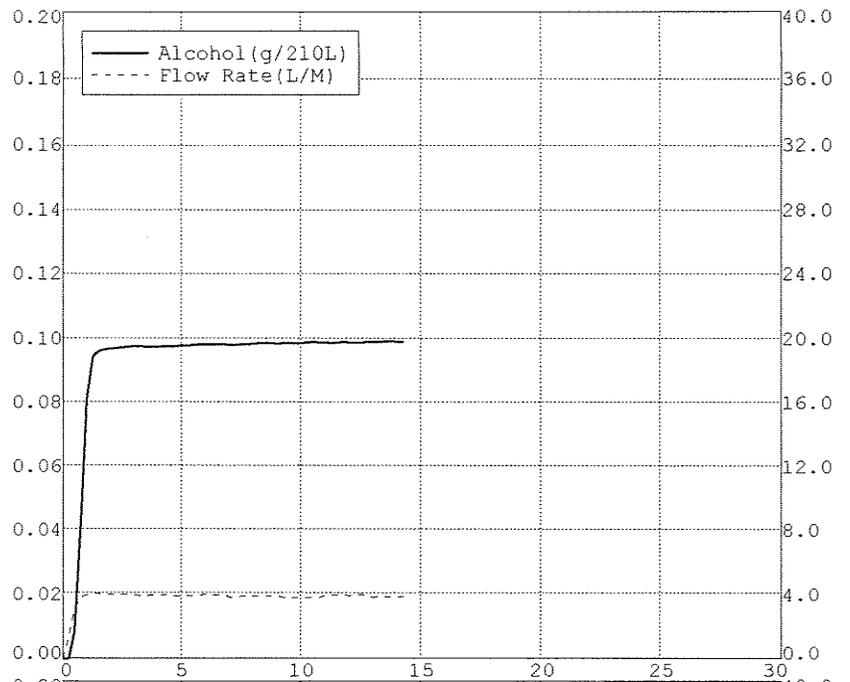

Handwritten signatures and initials:
A. M. 13. [Signature] # 2016