

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 02/01/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:47
INTERNAL STANDARD	VERIFIED	12:48
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:48
BLANK TEST	0.00	12:49
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:49
BLANK TEST	0.00	12:50
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:50
BLANK TEST	0.00	12:51

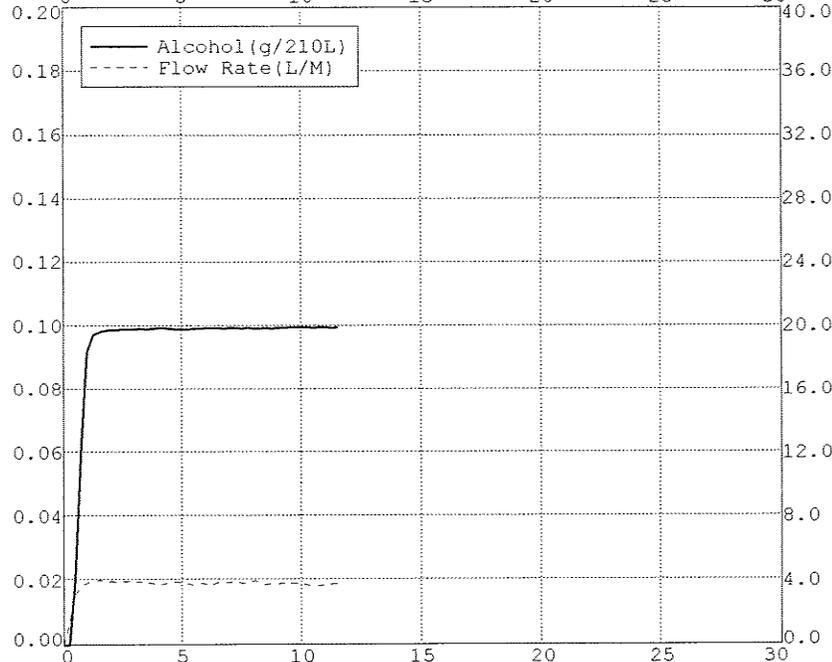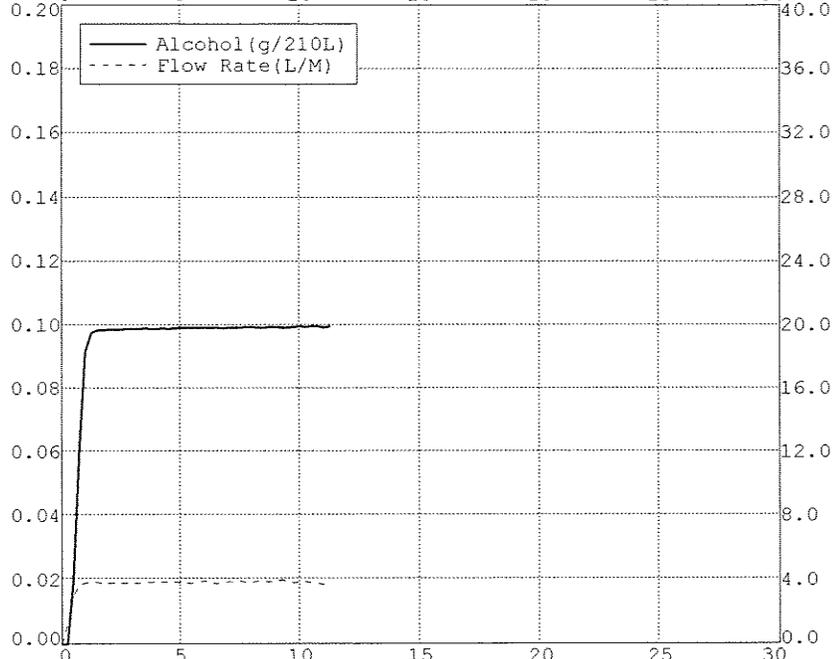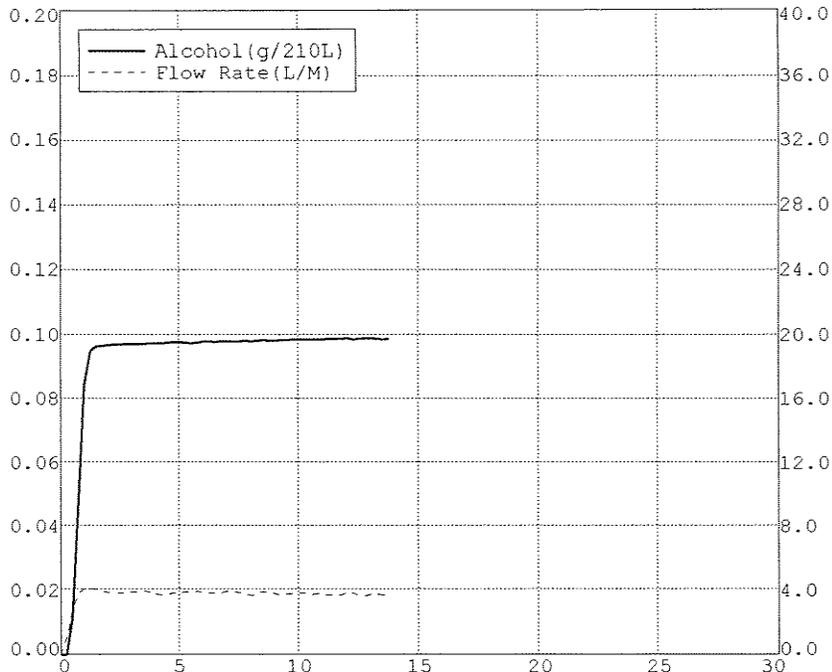

Signature: Sgt. Charles B. Geisler