

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 02/06/2020

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:34
INTERNAL STANDARD	VERIFIED	13:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:35
BLANK TEST	0.00	13:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:36
BLANK TEST	0.00	13:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:37
BLANK TEST	0.00	13:38

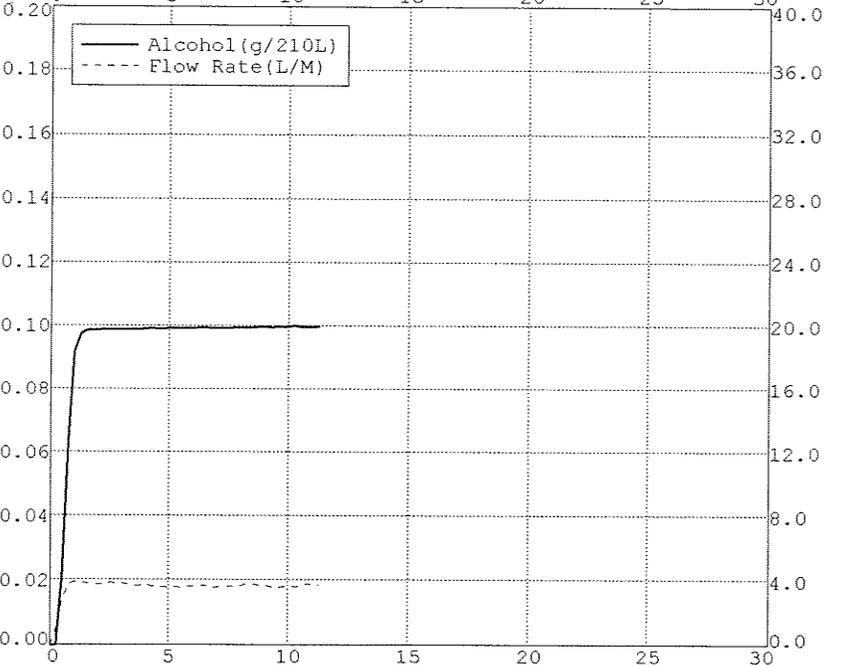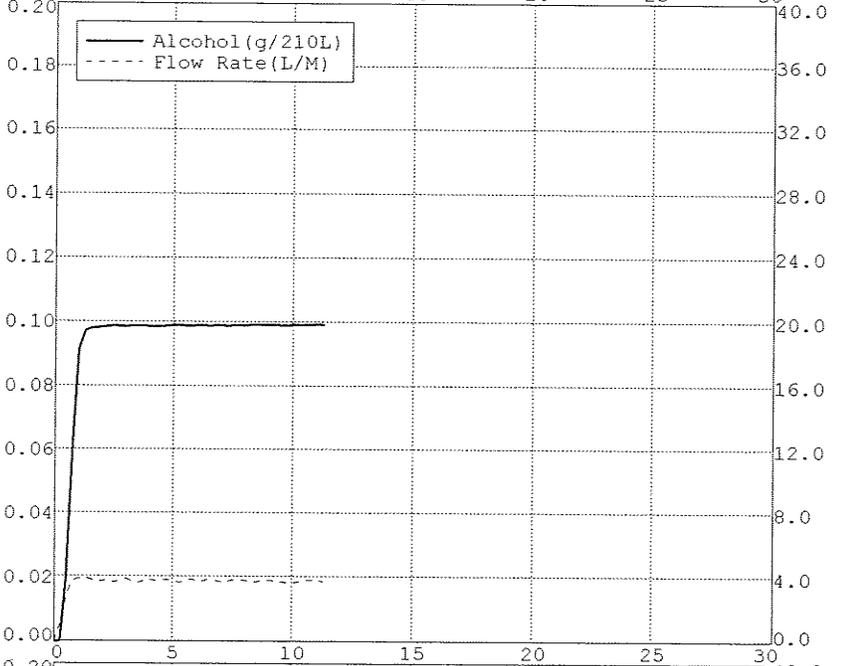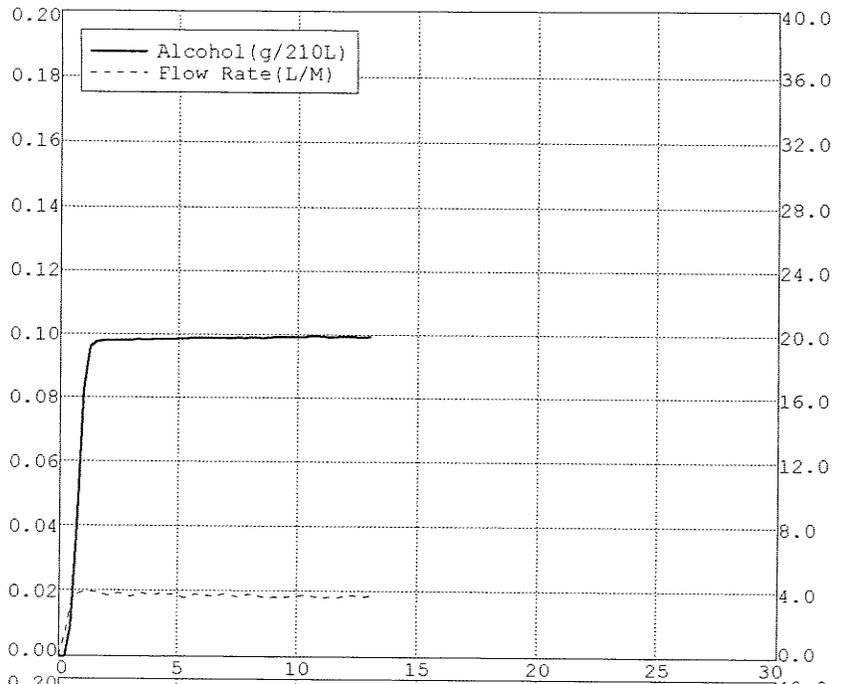

*Handwritten signature: Charles B. Geisler*