

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 02/14/2020

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:37
INTERNAL STANDARD	VERIFIED	13:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:37
BLANK TEST	0.00	13:38
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:38
BLANK TEST	0.00	13:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:40
BLANK TEST	0.00	13:40

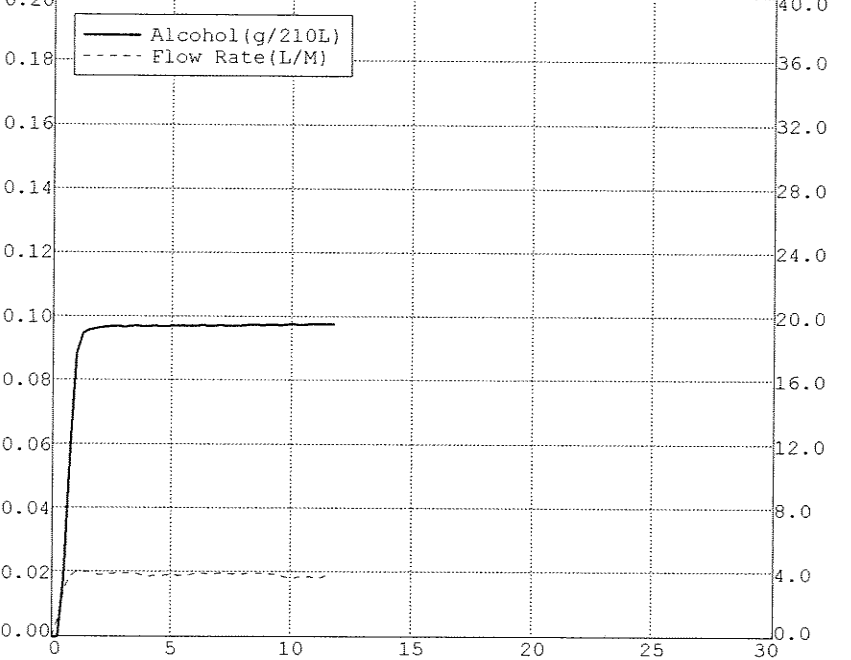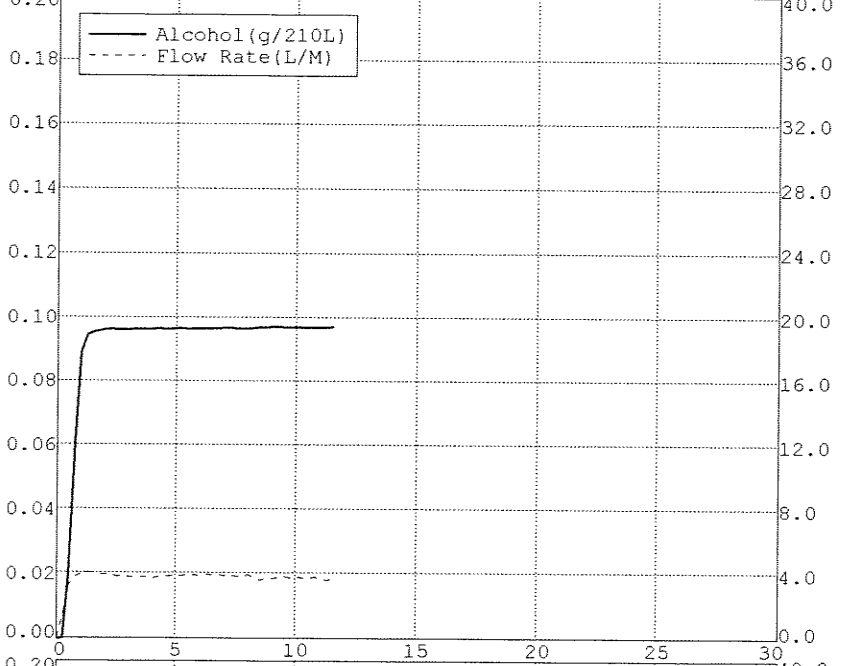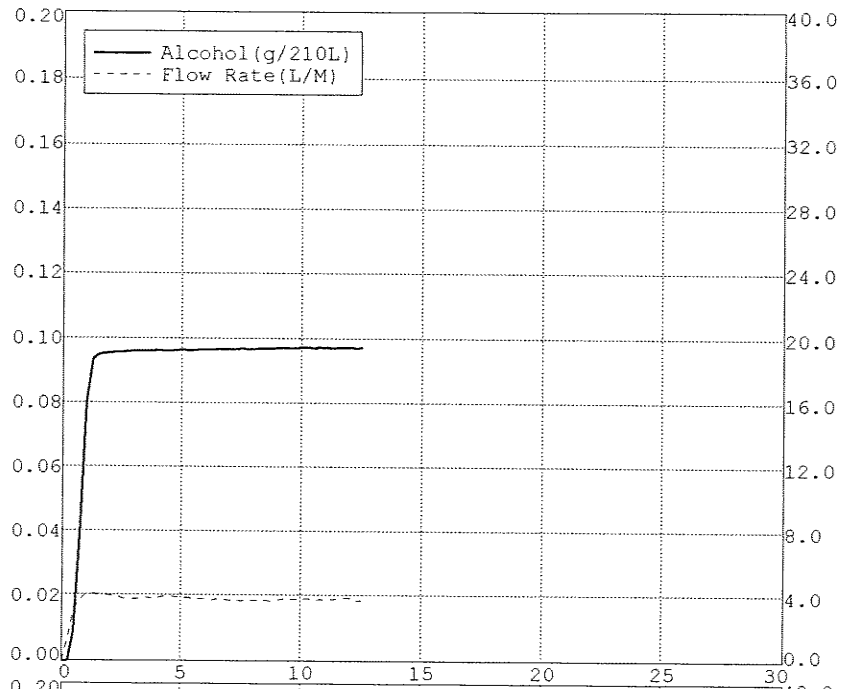

*Sgt. C. B. Geisler*  
*[Signature]*  
#248