

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 02/28/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:39
INTERNAL STANDARD	VERIFIED	13:39
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:39
BLANK TEST	0.00	13:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:41
BLANK TEST	0.00	13:41
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:42
BLANK TEST	0.00	13:43

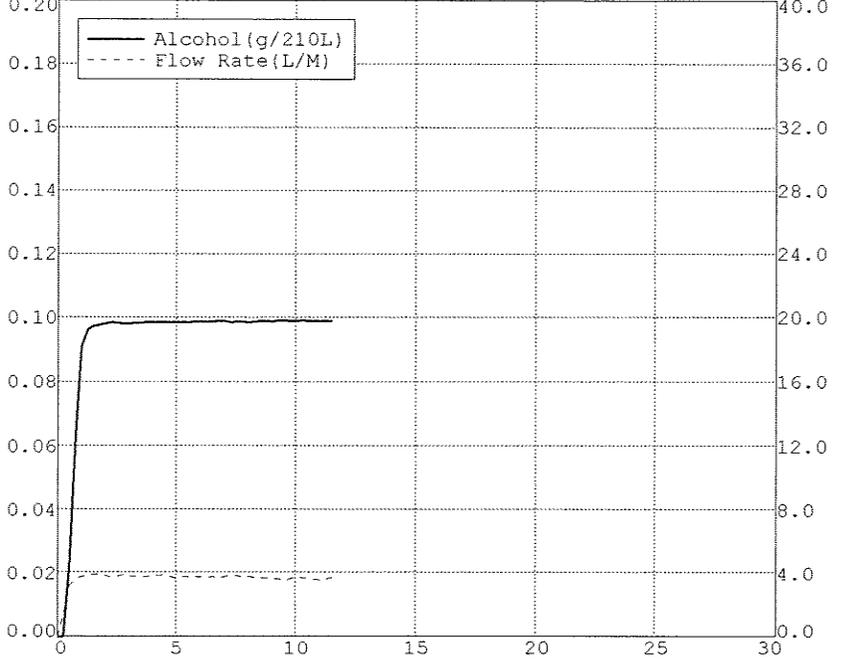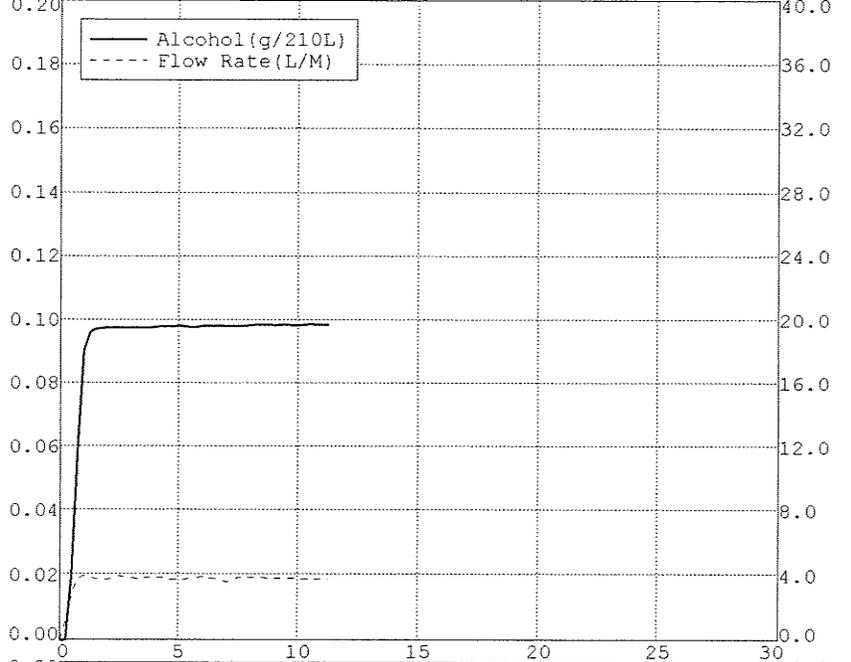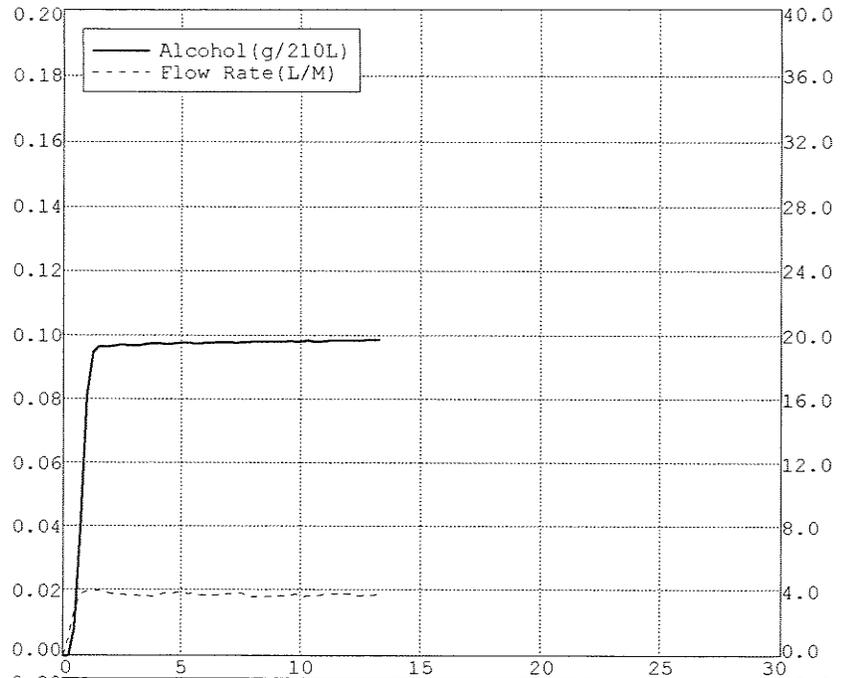

Sgt. Charles B. Geisler