

SUPERVISOR TEST




WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 105208

Date: 04/15/2020

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:56
INTERNAL STANDARD	VERIFIED	11:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:57
BLANK TEST	0.00	11:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:58
BLANK TEST	0.00	11:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:59
BLANK TEST	0.00	12:00

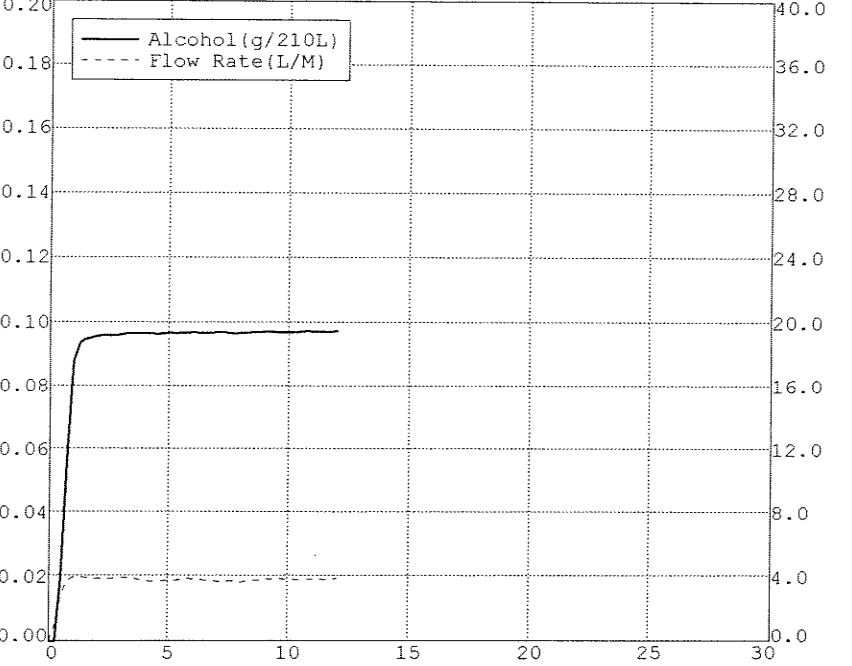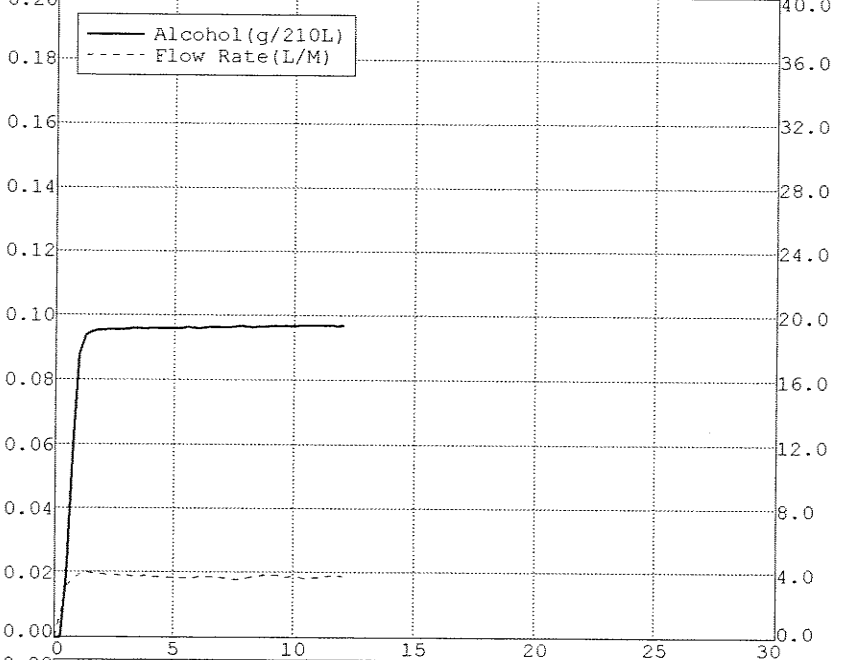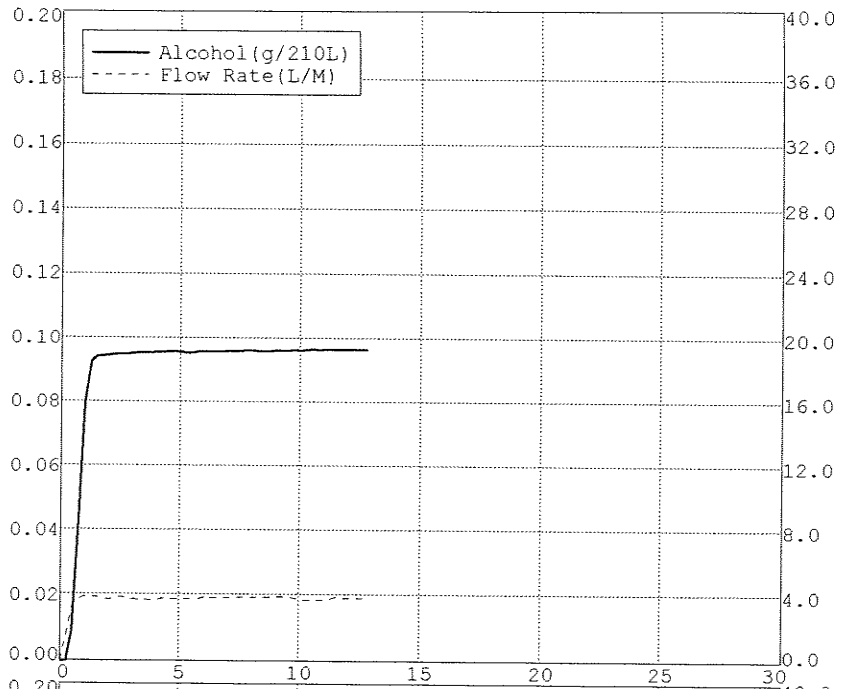

*Sgt. Charles B. Geisler #2010*