

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 04/30/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:42
INTERNAL STANDARD	VERIFIED	11:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:42
BLANK TEST	0.00	11:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:43
BLANK TEST	0.00	11:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:44
BLANK TEST	0.00	11:45

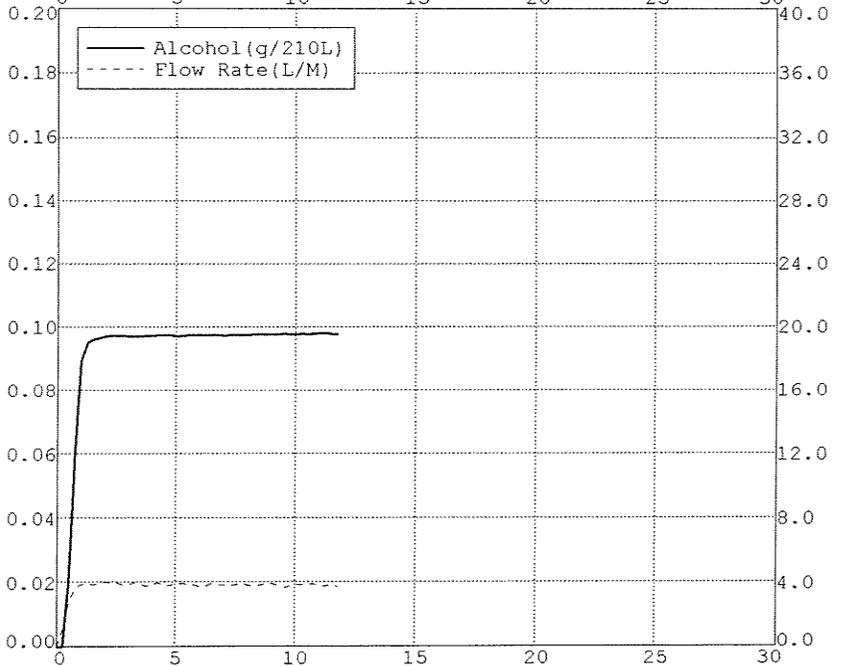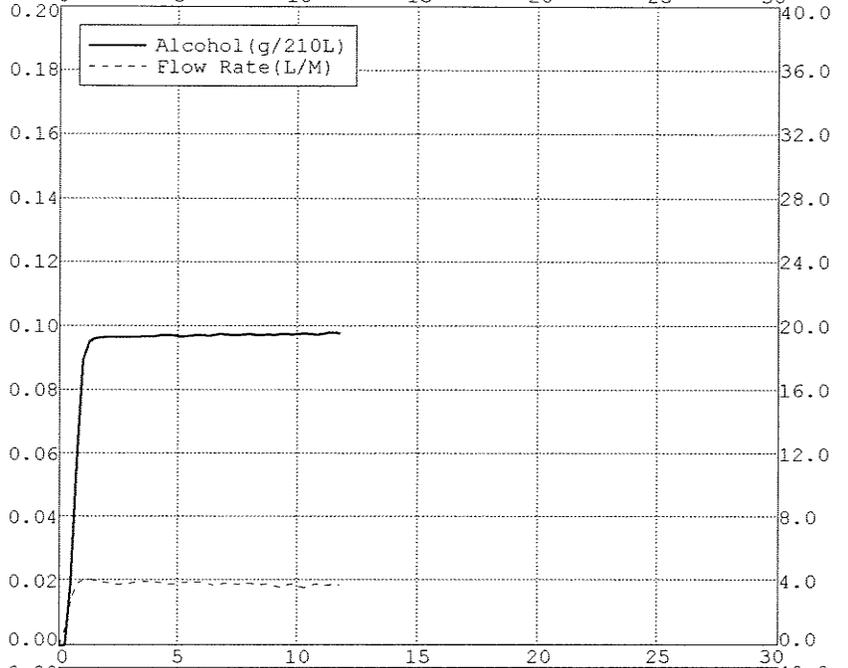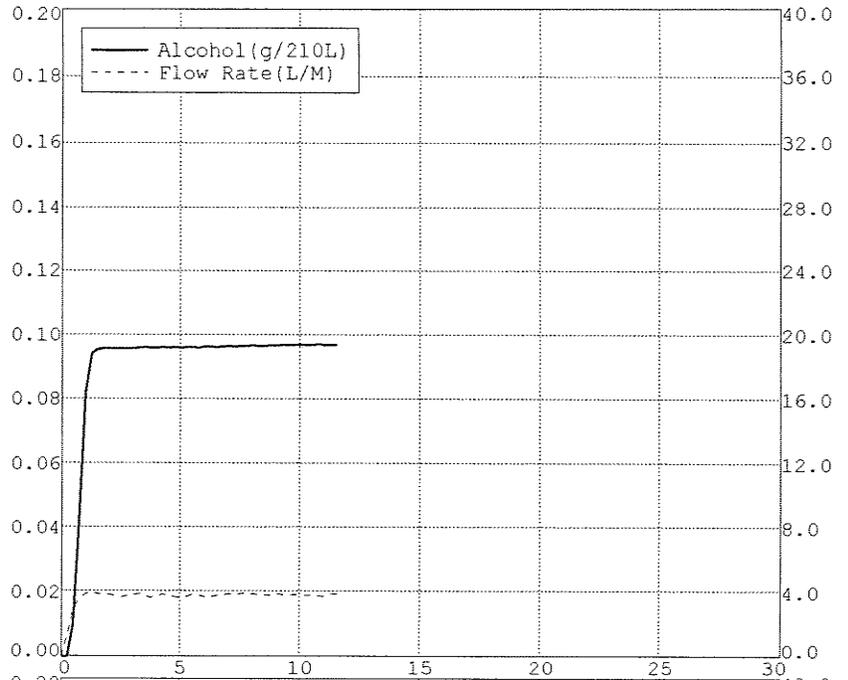

Signature: Sgt. Charles B. Geisler