

SUPERVISOR TEST




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208

Date: 05/06/2020

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:33
INTERNAL STANDARD	VERIFIED	12:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:33
BLANK TEST	0.00	12:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:34
BLANK TEST	0.00	12:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:35
BLANK TEST	0.00	12:36

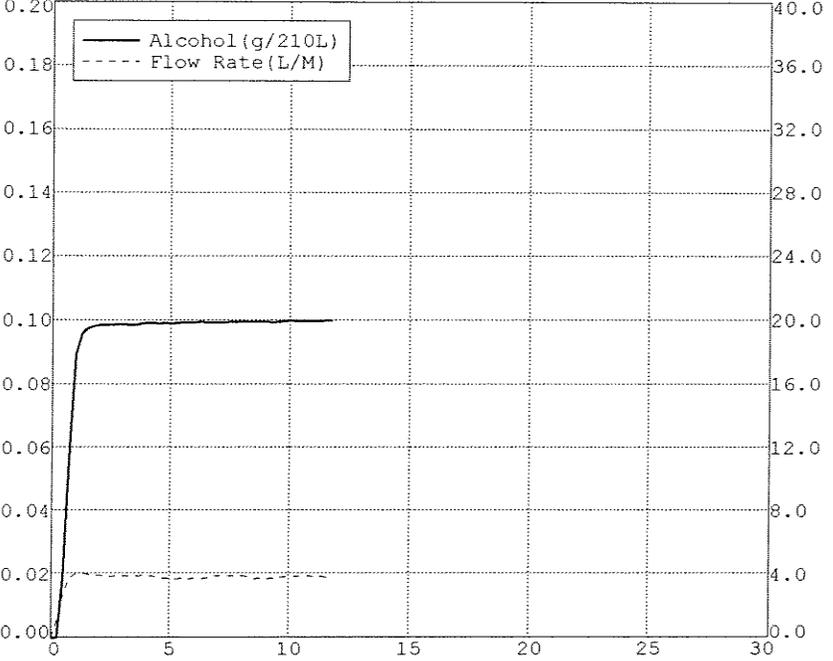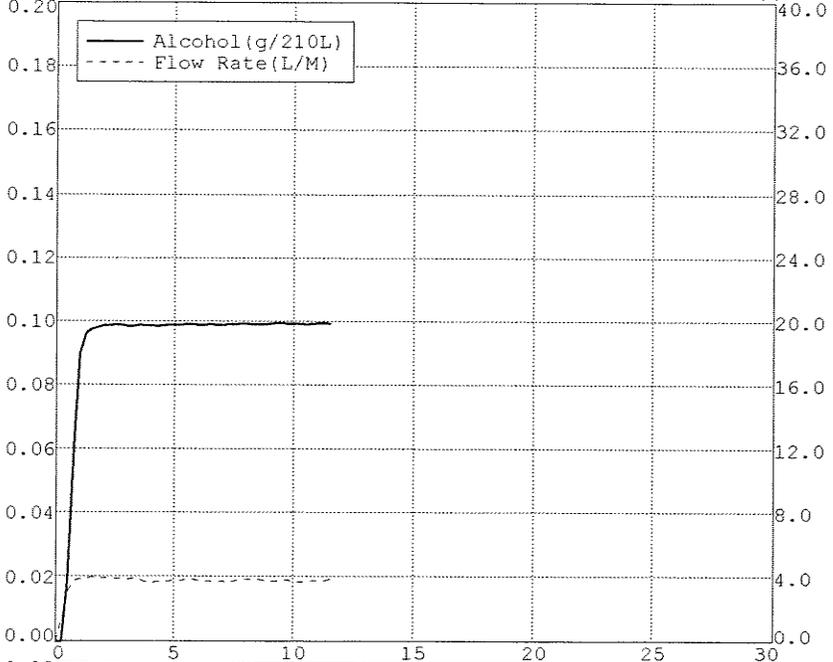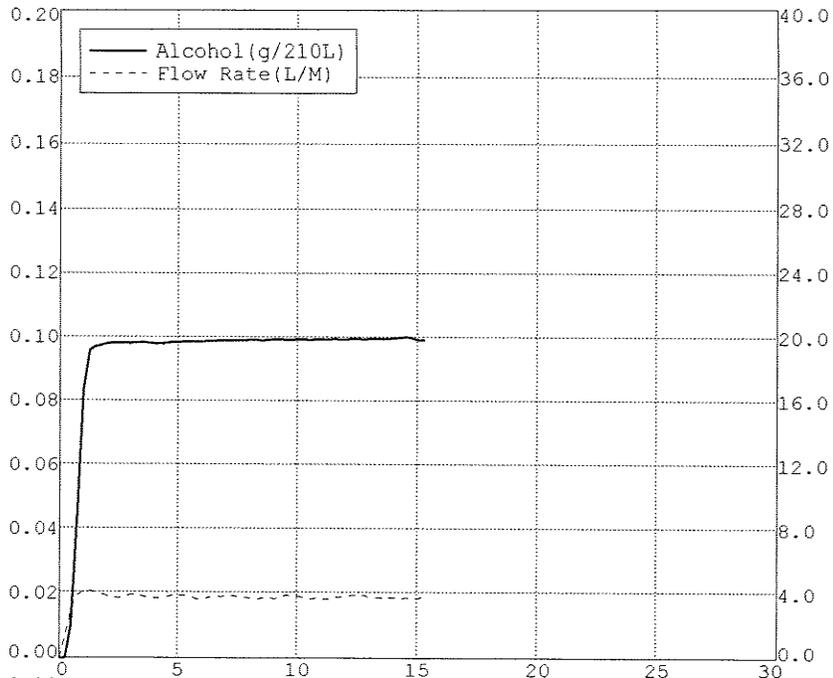

Sgt. Charles B. Geisler