

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 05/27/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:44
INTERNAL STANDARD	VERIFIED	13:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:44
BLANK TEST	0.00	13:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	13:45
BLANK TEST	0.00	13:46
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	13:46
BLANK TEST	0.00	13:47

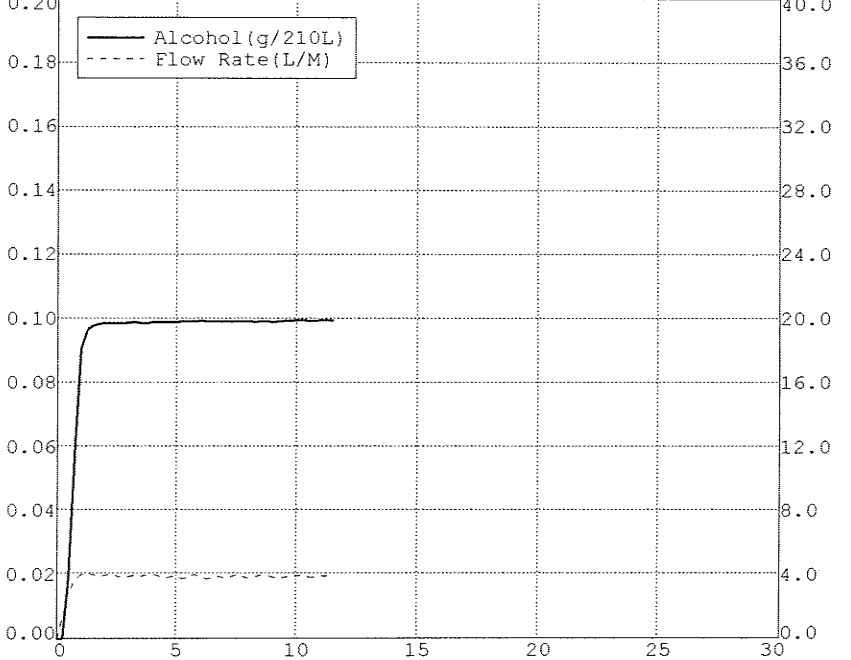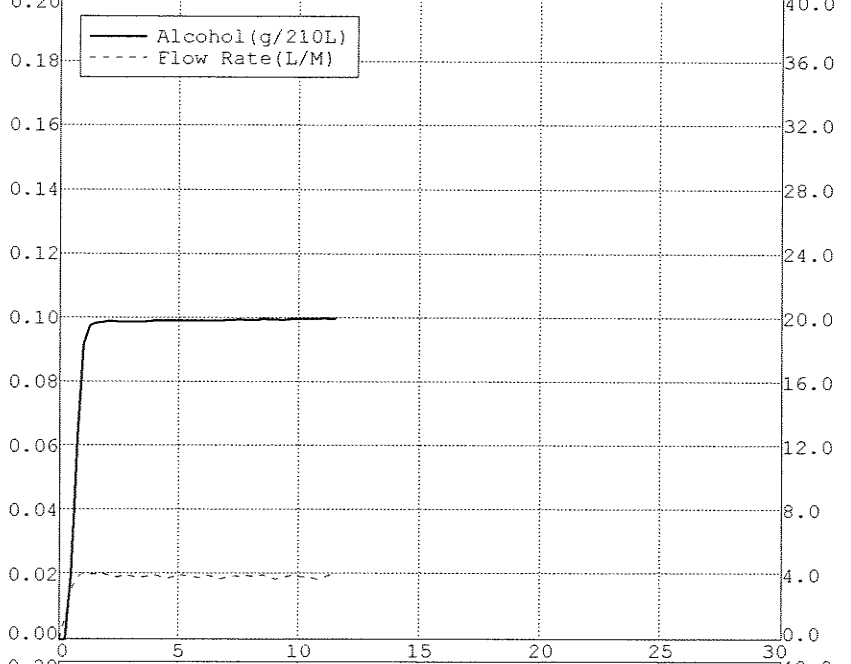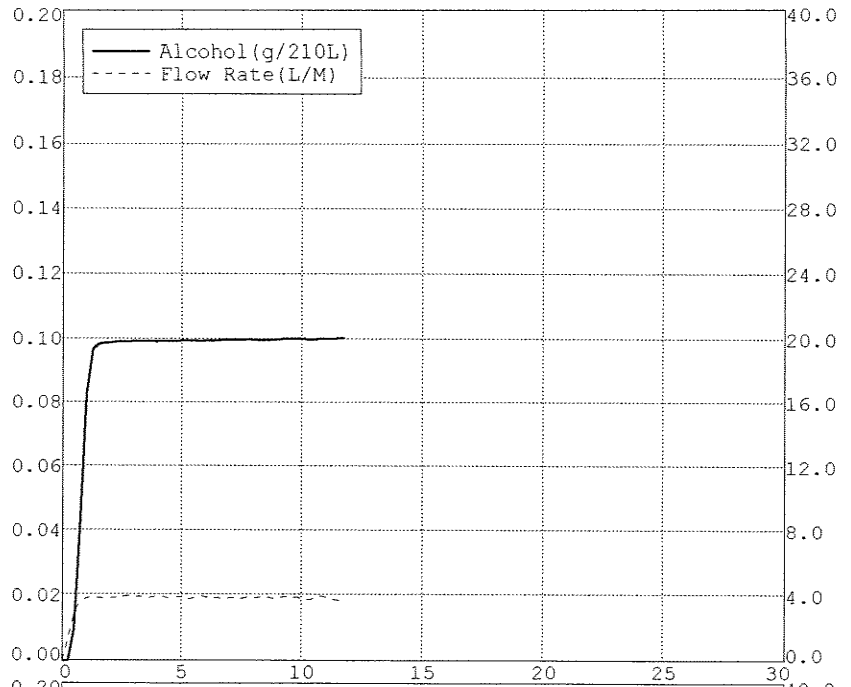

Sgt. Charles B. Geisler