

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 06/02/2020

OPERATOR NAME:
MICHAEL A CAMPBELL
Permit #: 42422
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:16
INTERNAL STANDARD	VERIFIED	05:16
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	05:17
BLANK TEST	0.00	05:18
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	05:18
BLANK TEST	0.00	05:19
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	05:19
BLANK TEST	0.00	05:20

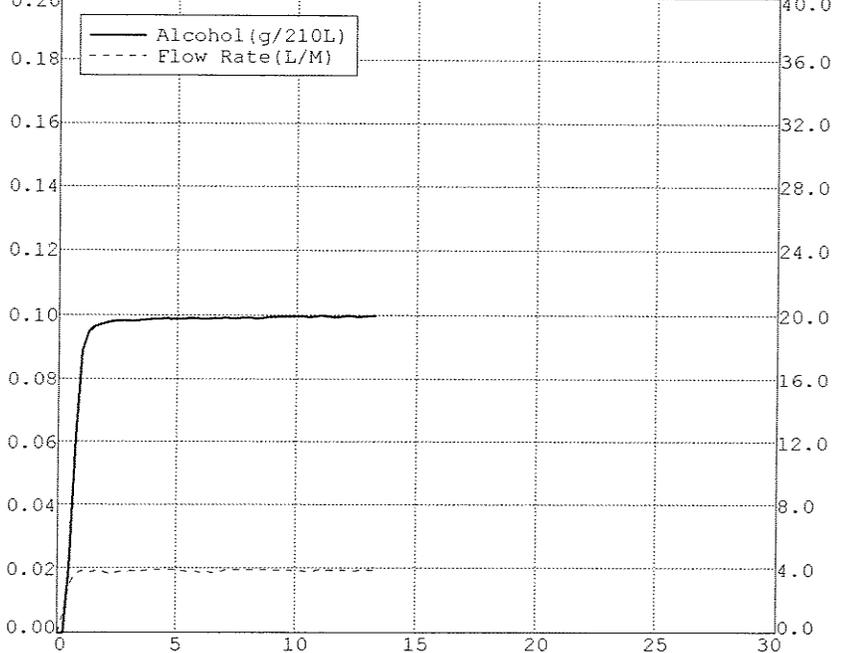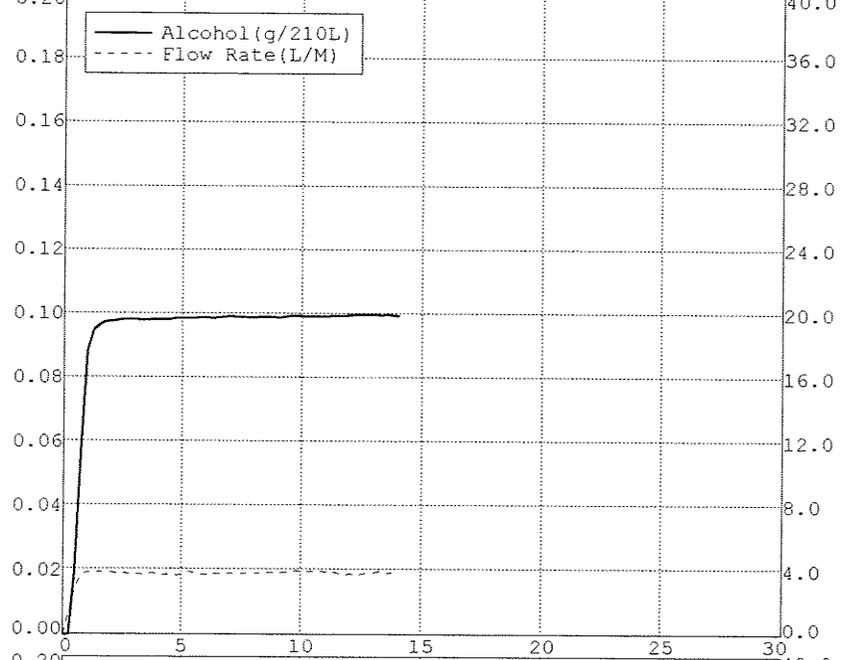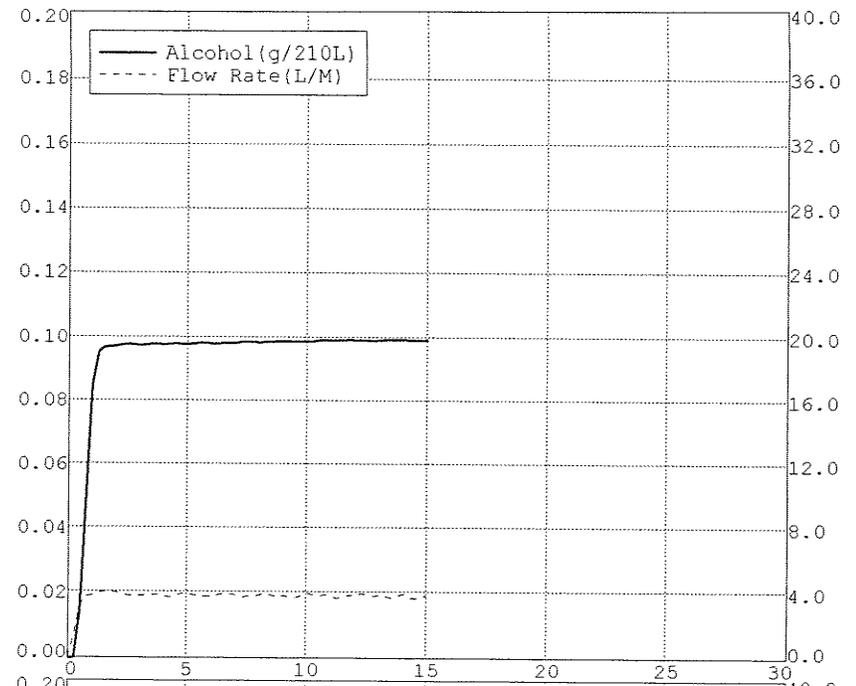

Michael A Campbell #157