

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 06/15/2020

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:13
INTERNAL STANDARD	VERIFIED	14:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:13
BLANK TEST	0.00	14:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:14
BLANK TEST	0.00	14:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:16
BLANK TEST	0.00	14:16

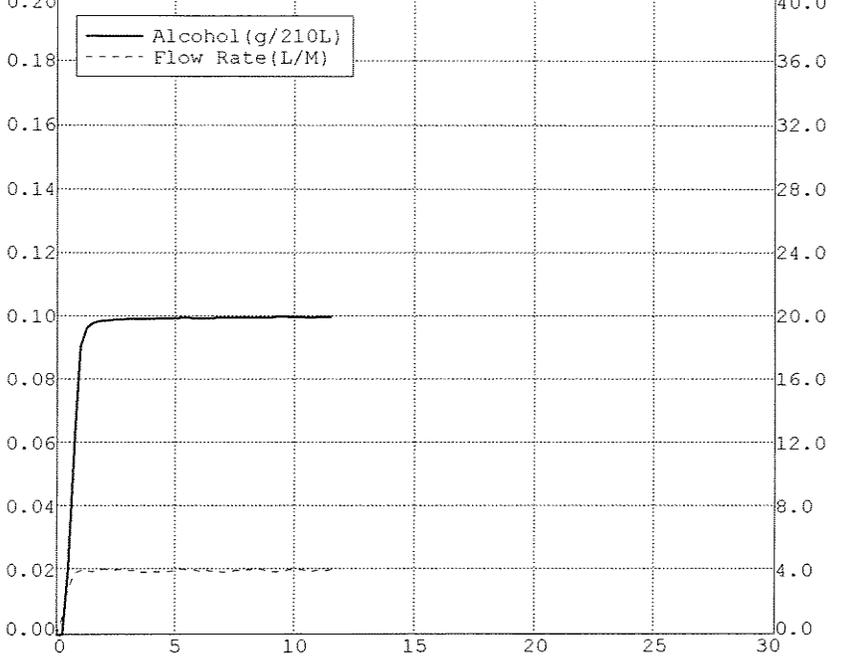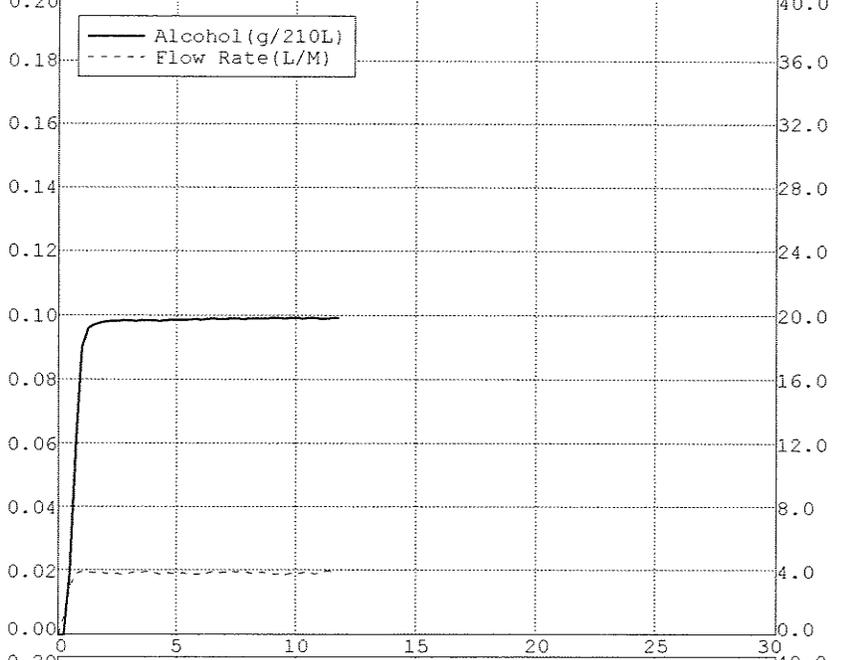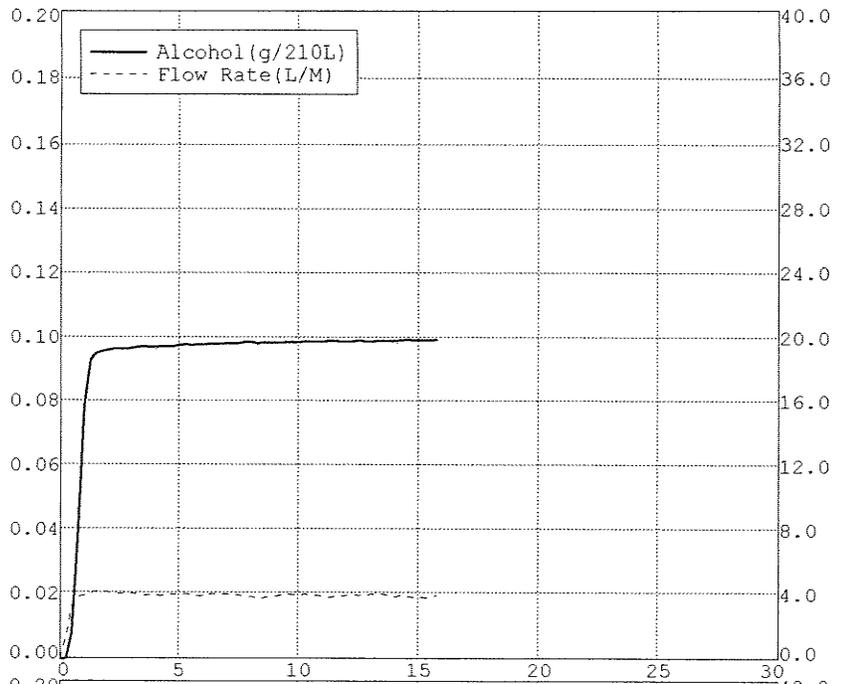

*Charles B. Geisler*