

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 06/21/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:21
INTERNAL STANDARD	VERIFIED	16:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:21
BLANK TEST	0.00	16:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:22
BLANK TEST	0.00	16:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:23
BLANK TEST	0.00	16:24

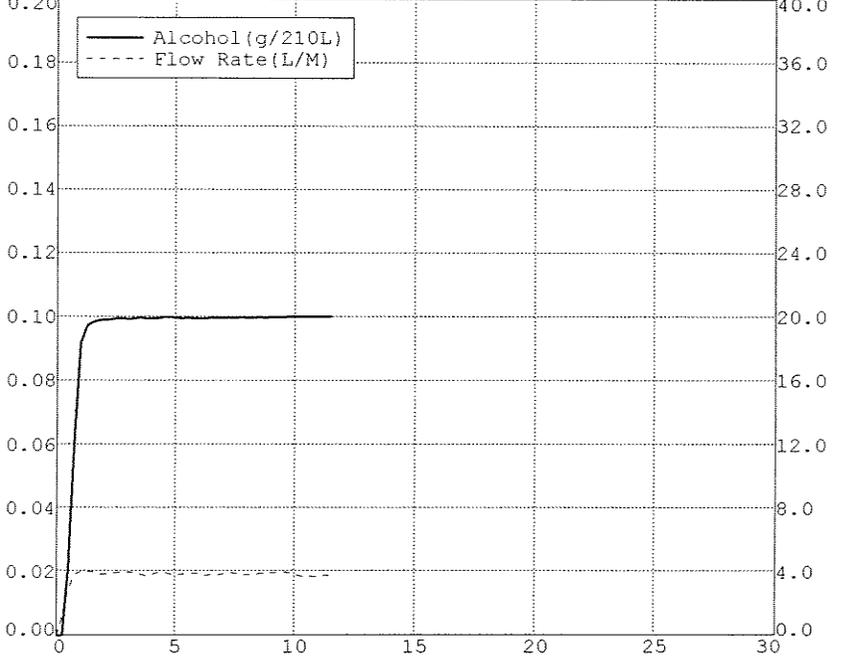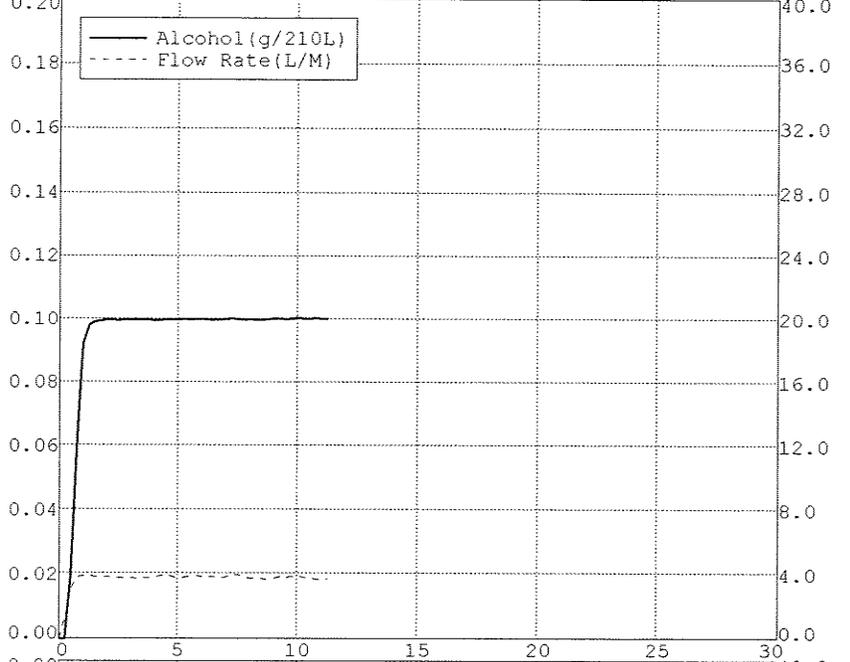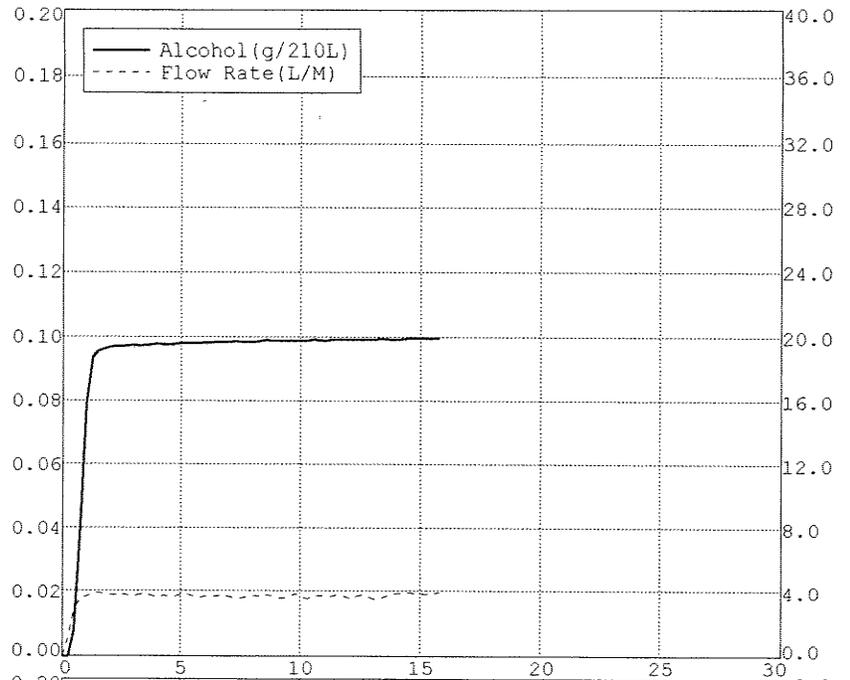

Sgt. M. B. Geisler