

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 06/29/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:57
INTERNAL STANDARD	VERIFIED	12:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:57
BLANK TEST	0.00	12:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:58
BLANK TEST	0.00	12:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	12:59
BLANK TEST	0.00	13:00

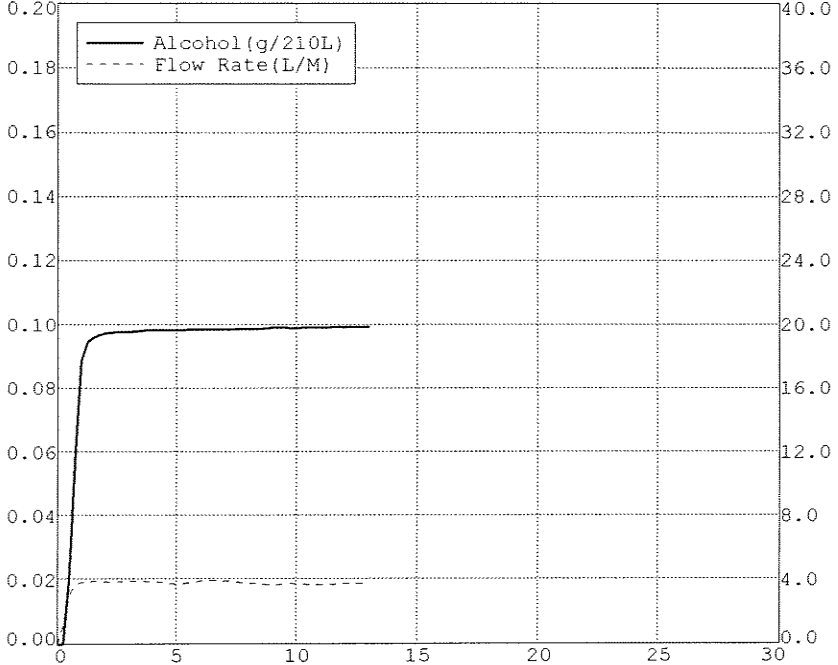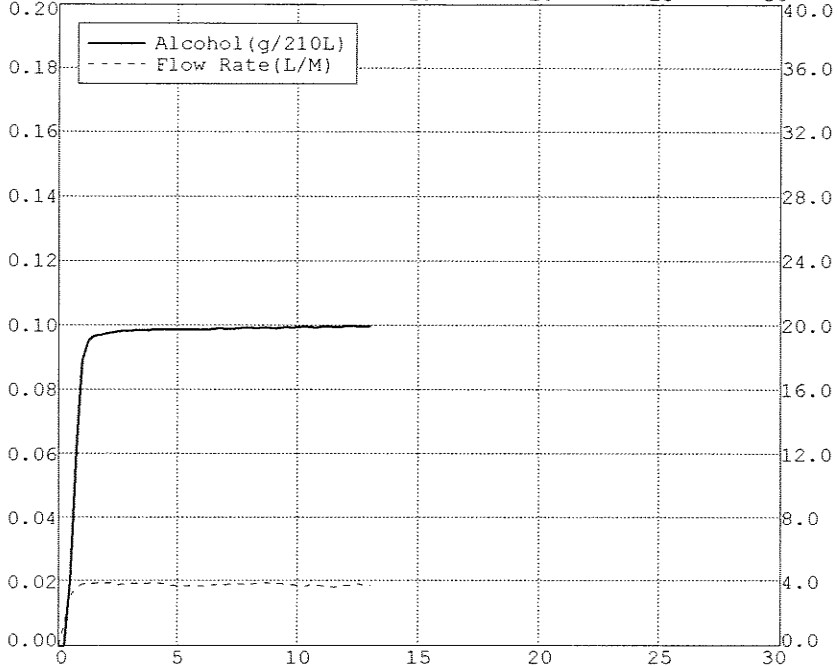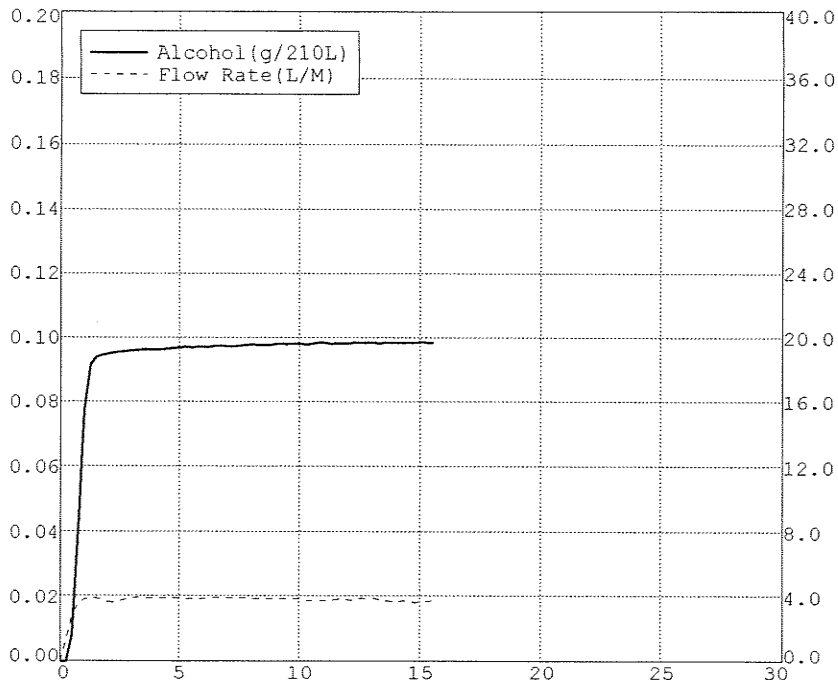

Handwritten signatures and initials:
J. Allen - B. [Signature] #2nd