

SOLUTION CHANGE




WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 105208

Date: 07/03/2020

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:58
INTERNAL STANDARD	VERIFIED	15:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:59
BLANK TEST	0.00	15:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:00
BLANK TEST	0.00	16:01
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:01
BLANK TEST	0.00	16:02

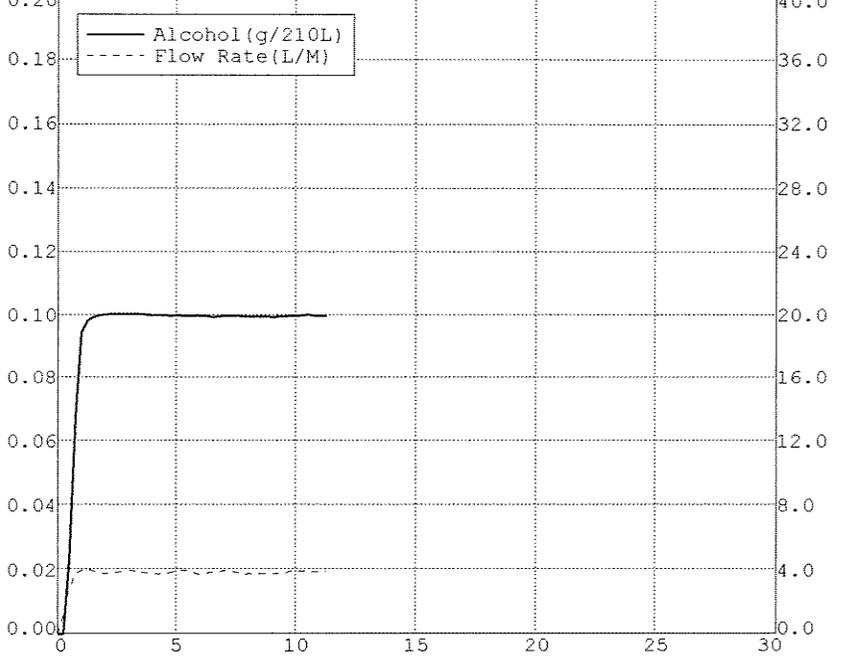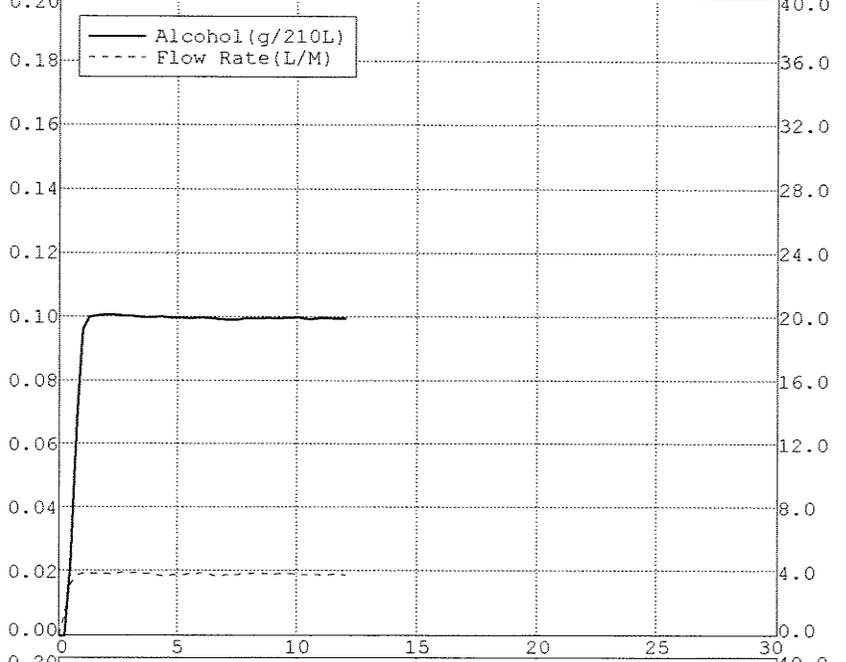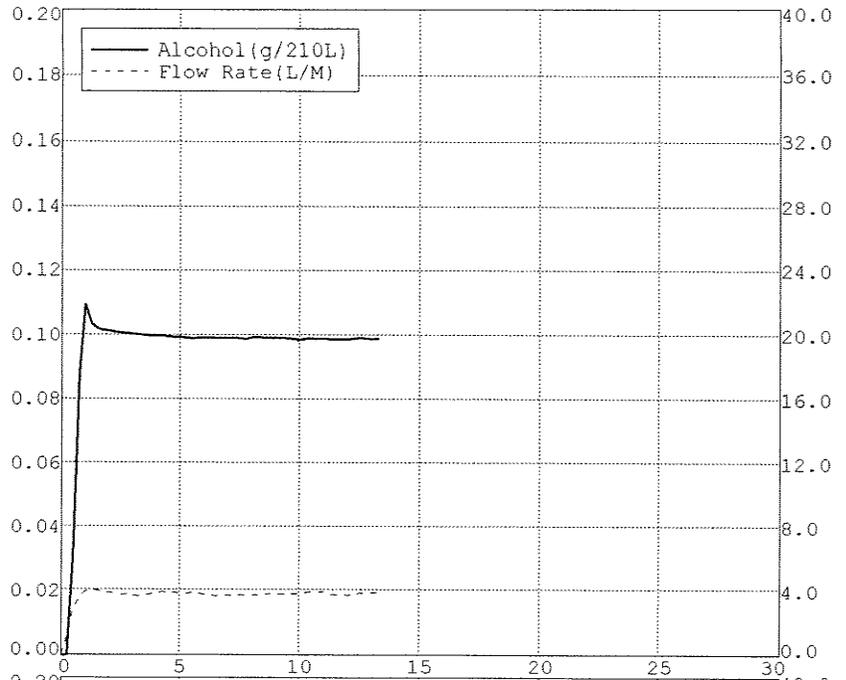

*Signature: Charles B. Geisler*