

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 07/07/2020

OPERATOR NAME:  
TYLER J MORSE  
Permit #: 41959  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:04
INTERNAL STANDARD	VERIFIED	17:04
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	17:05
BLANK TEST	0.00	17:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	17:06
BLANK TEST	0.00	17:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	17:07
BLANK TEST	0.00	17:08

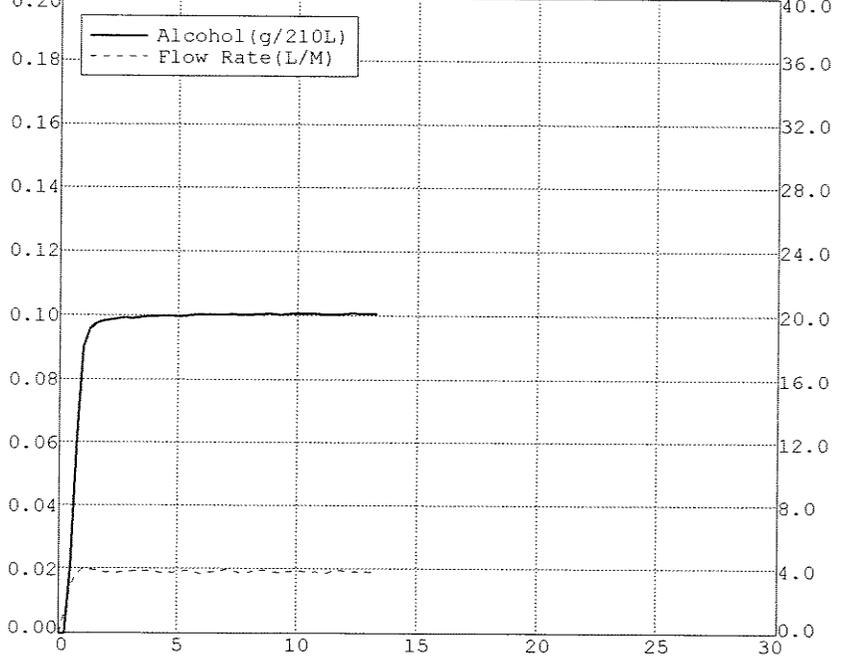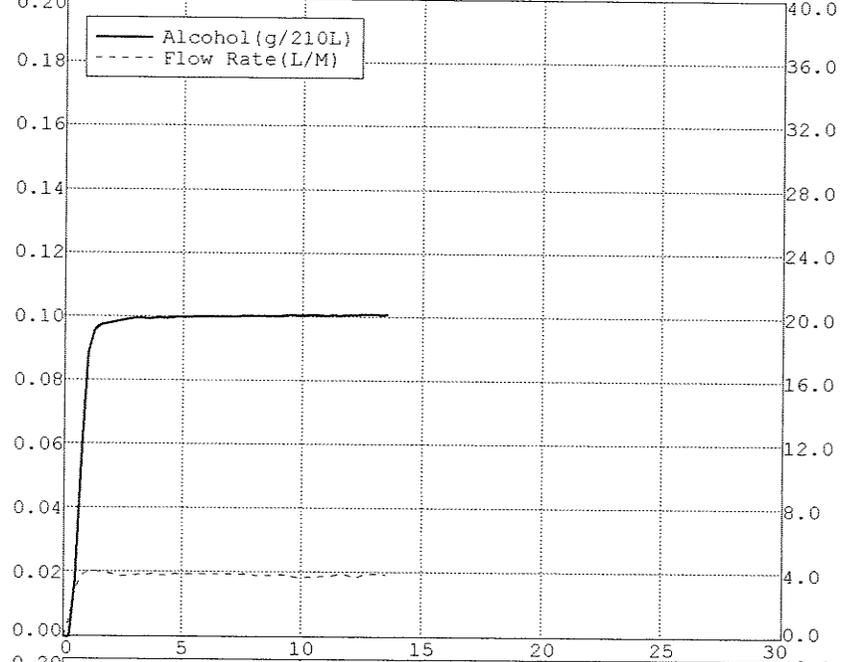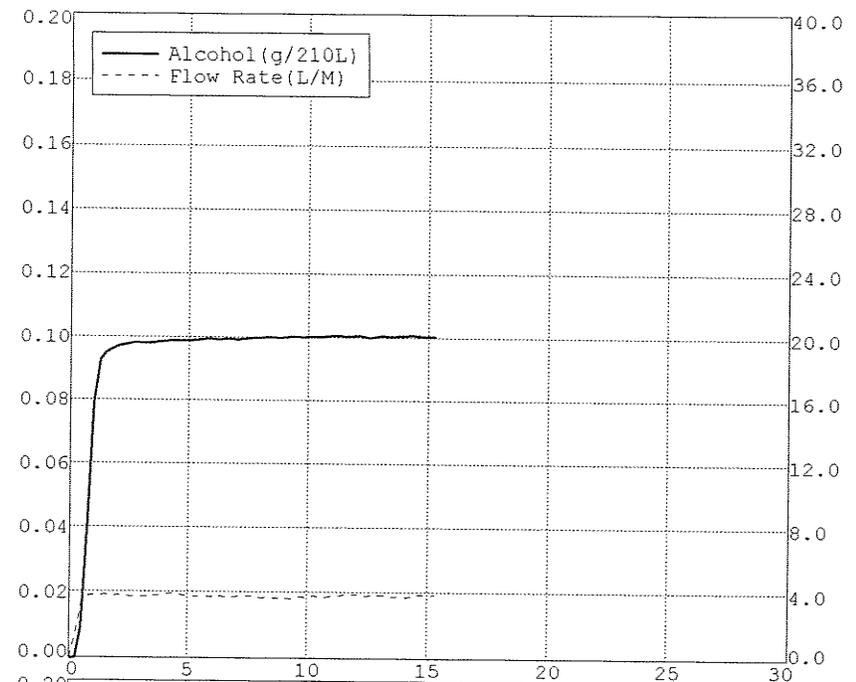

*Handwritten signature and number: #447*

*Handwritten text: ps morse*