

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 07/22/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:56
INTERNAL STANDARD	VERIFIED	16:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:56
BLANK TEST	0.00	16:57
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:58
BLANK TEST	0.00	16:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	16:59
BLANK TEST	0.00	17:00

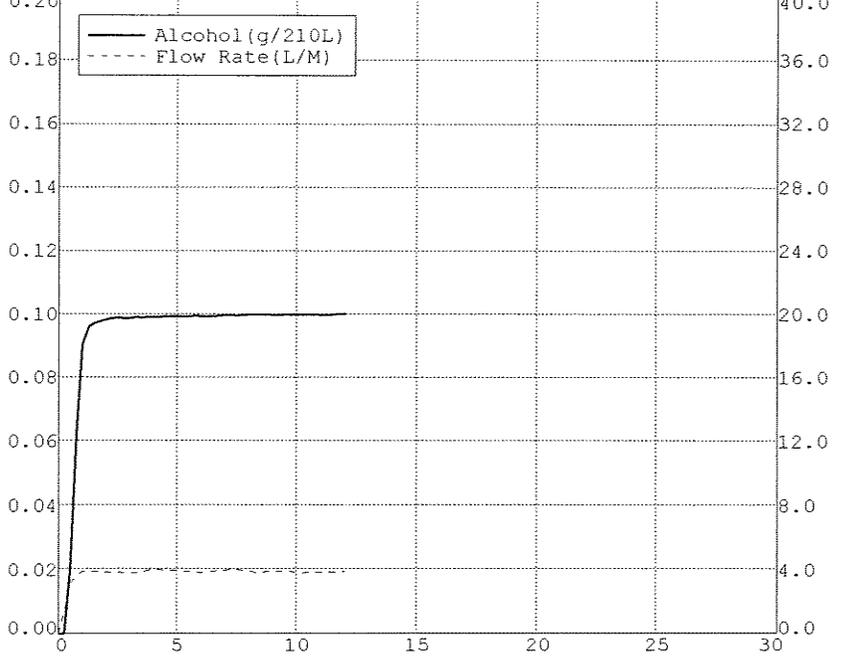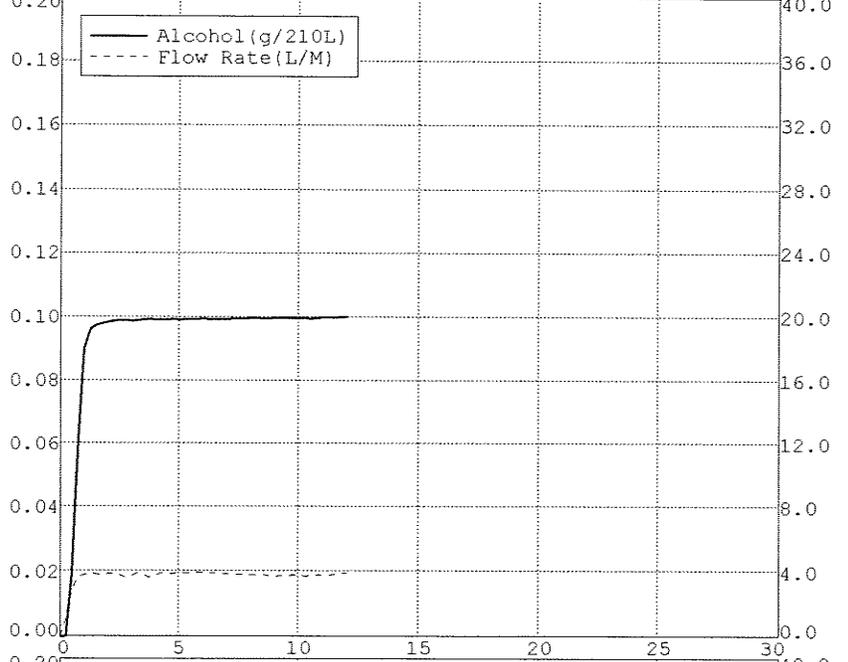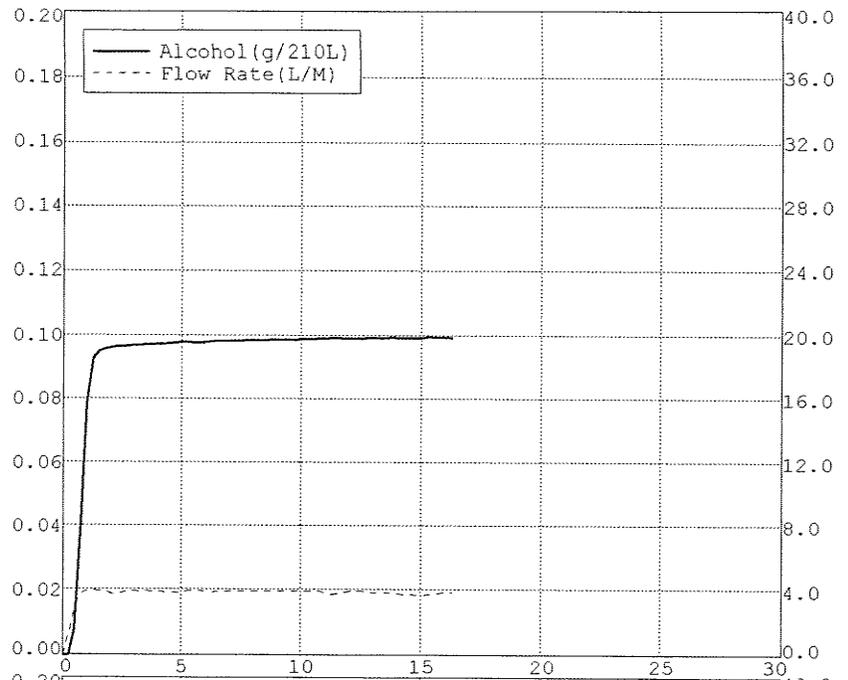

Ch. B. Geisler #201