

SUPERVISOR TEST




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 105208

Date: 08/06/2020

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:10
INTERNAL STANDARD	VERIFIED	15:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:11
BLANK TEST	0.00	15:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:12
BLANK TEST	0.00	15:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:13
BLANK TEST	0.00	15:14

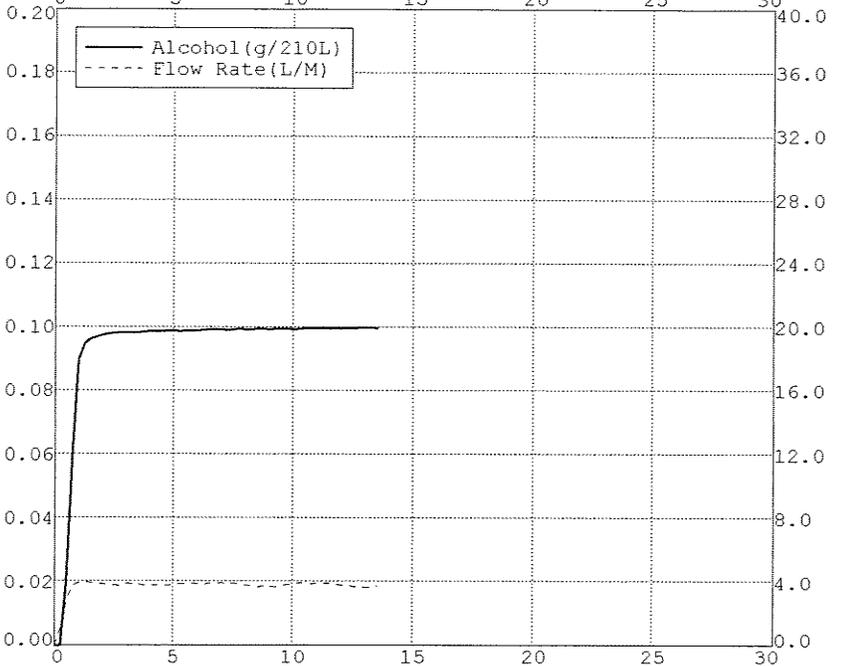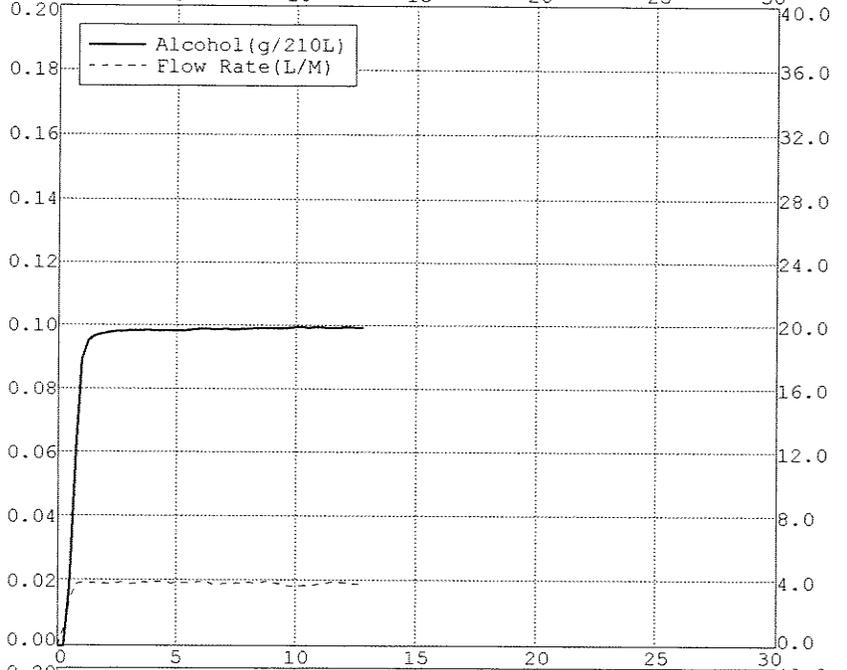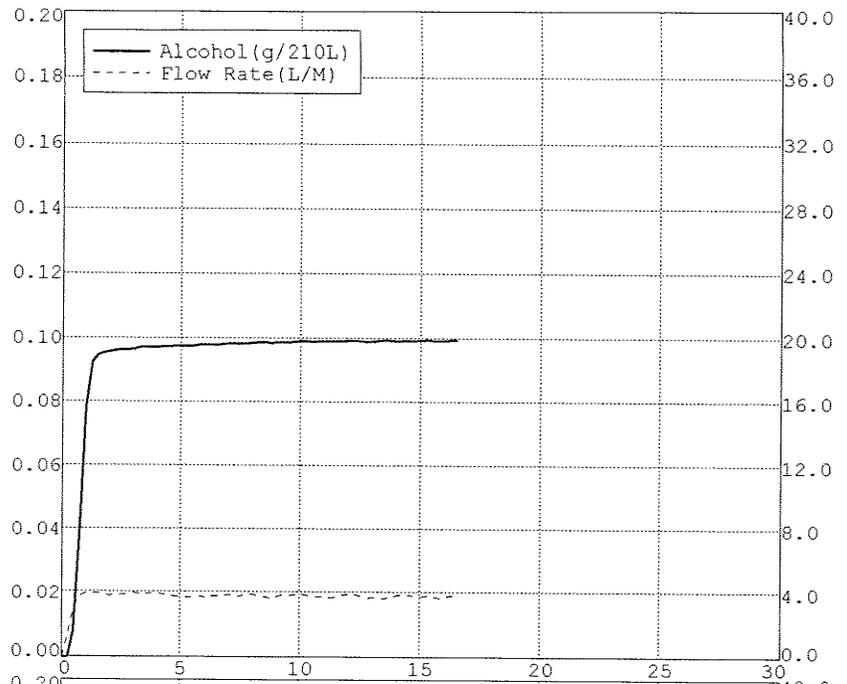

Handwritten signatures and initials:
 J. C. M. B. [Signature] [Signature]