

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 08/20/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:41
INTERNAL STANDARD	VERIFIED	14:41
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:42
BLANK TEST	0.00	14:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:43
BLANK TEST	0.00	14:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:44
BLANK TEST	0.00	14:45

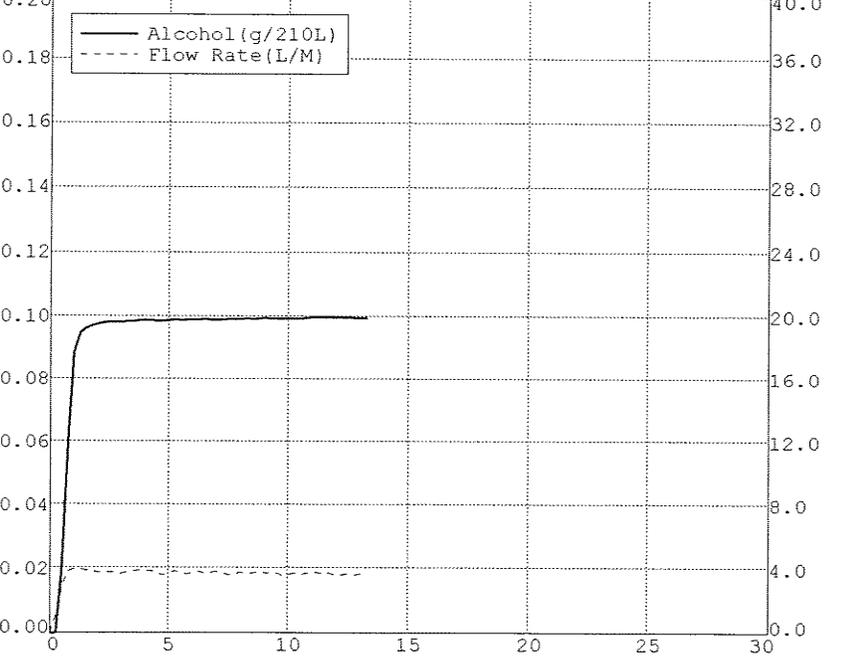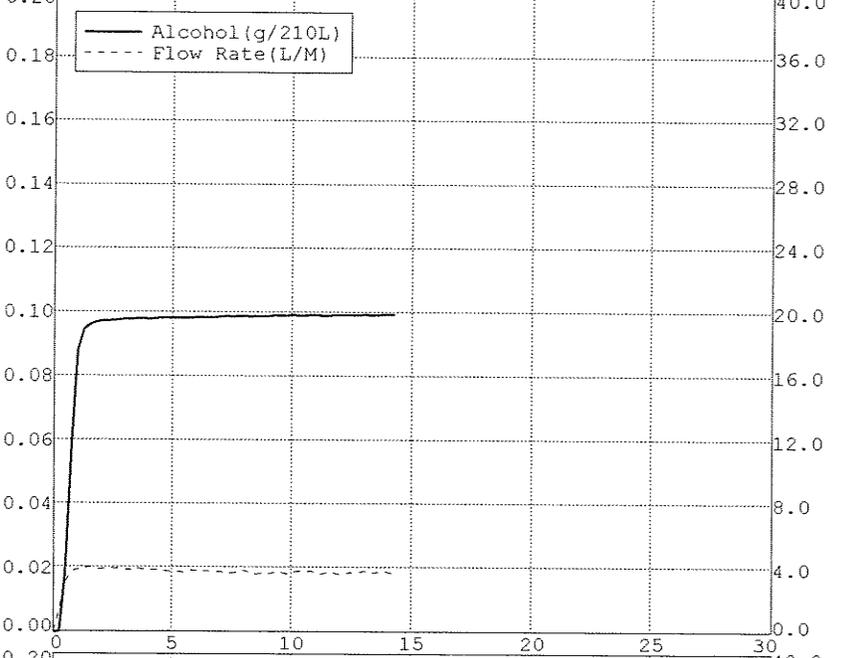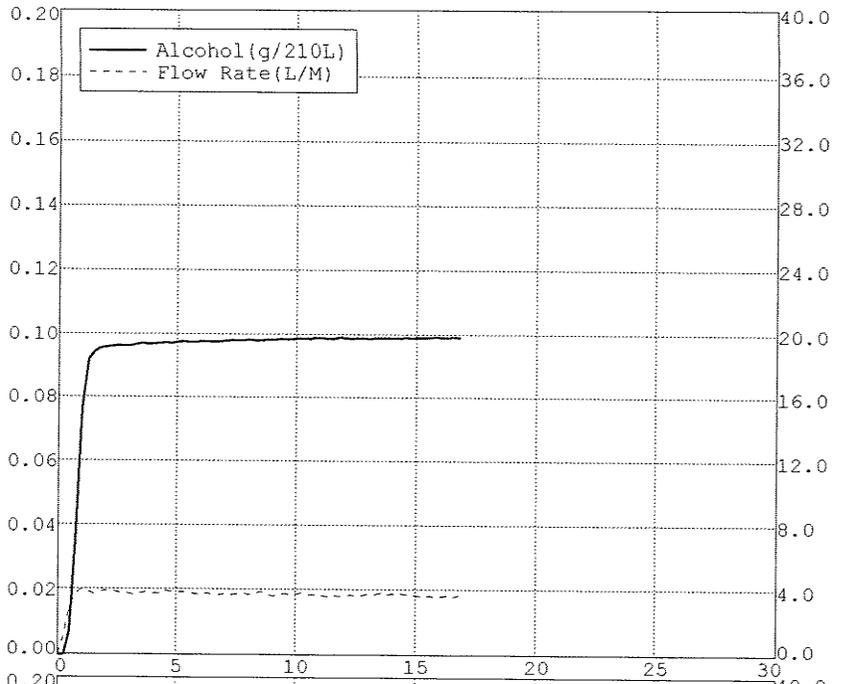

Sgt. Charles B. Geisler