

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 09/08/2020

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:40
INTERNAL STANDARD	VERIFIED	14:40
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:40
BLANK TEST	0.00	14:41
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:42
BLANK TEST	0.00	14:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	14:43
BLANK TEST	0.00	14:44

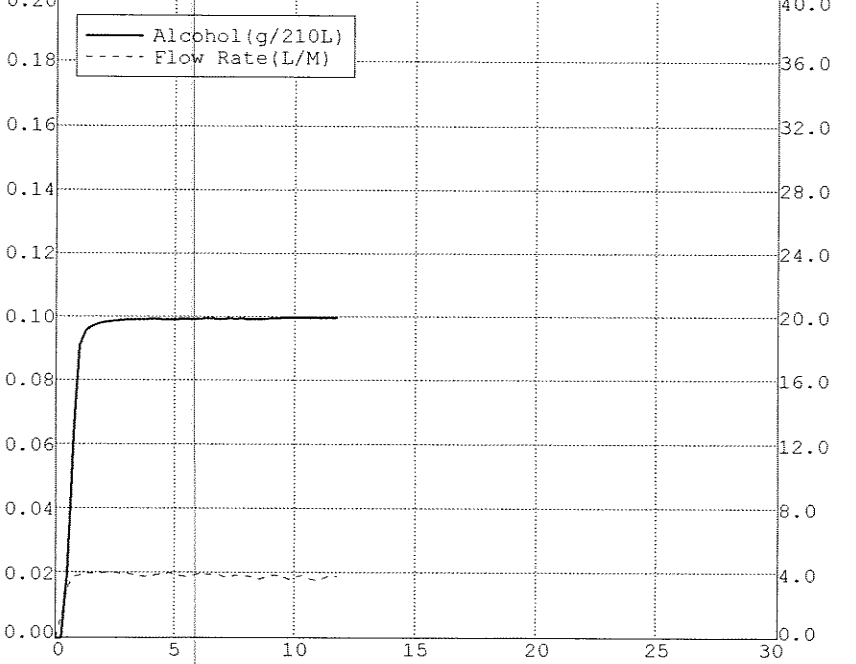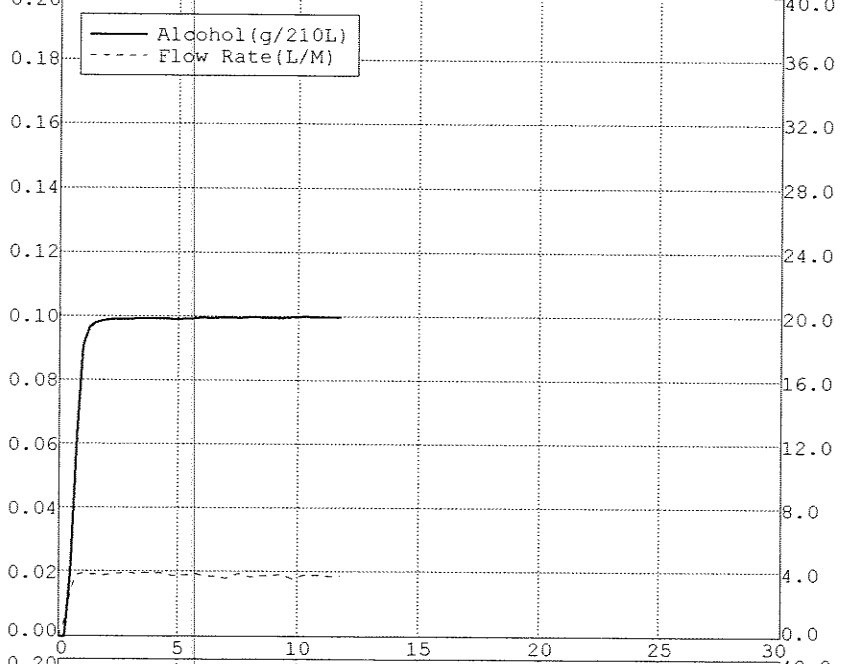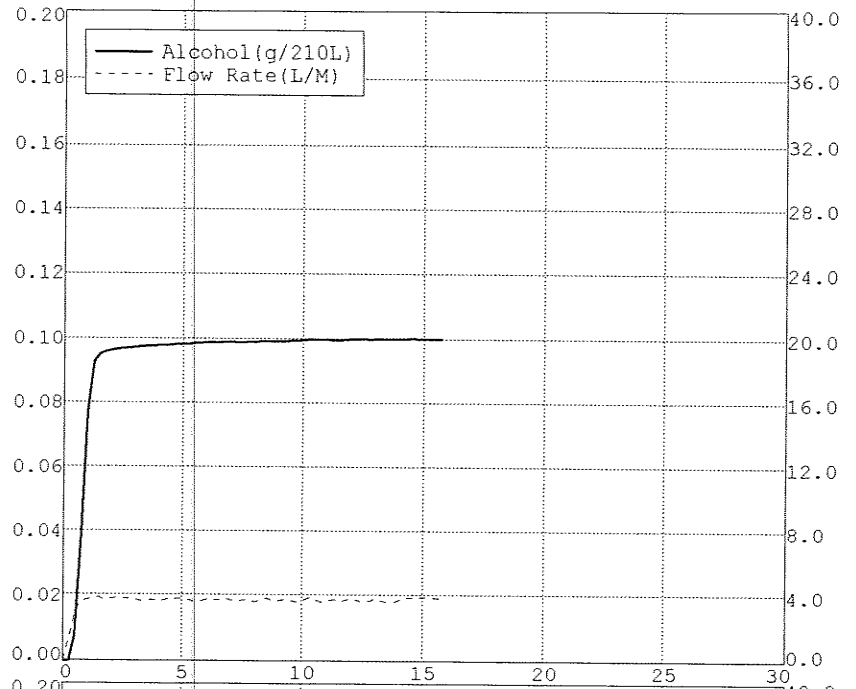

*Handwritten signatures:*  
C.B. Geisler  
[Signature]