

SUPERVISOR TEST




WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 105208

Date: 09/25/2020

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:28
INTERNAL STANDARD	VERIFIED	17:28
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	17:29
BLANK TEST	0.00	17:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	17:30
BLANK TEST	0.00	17:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	17:31
BLANK TEST	0.00	17:32

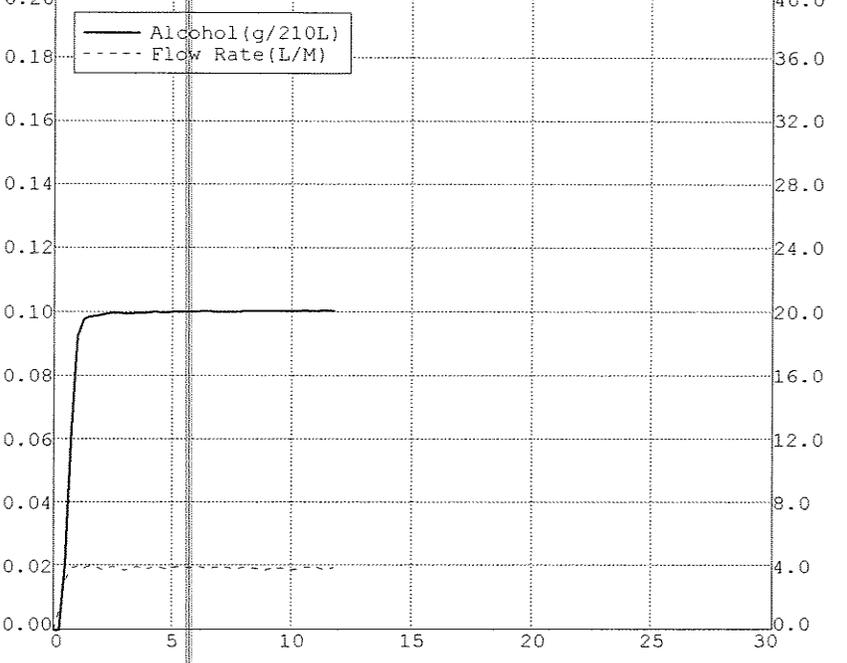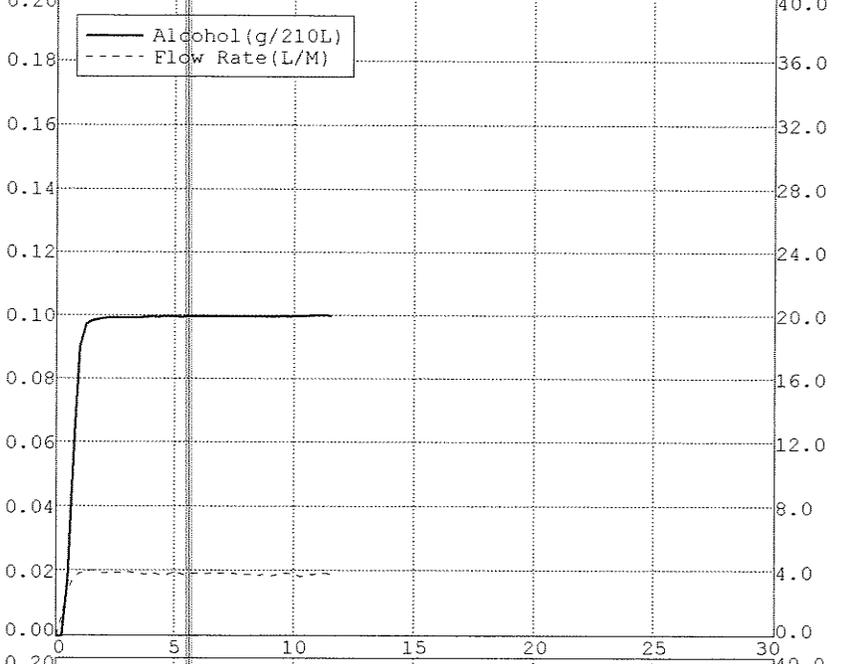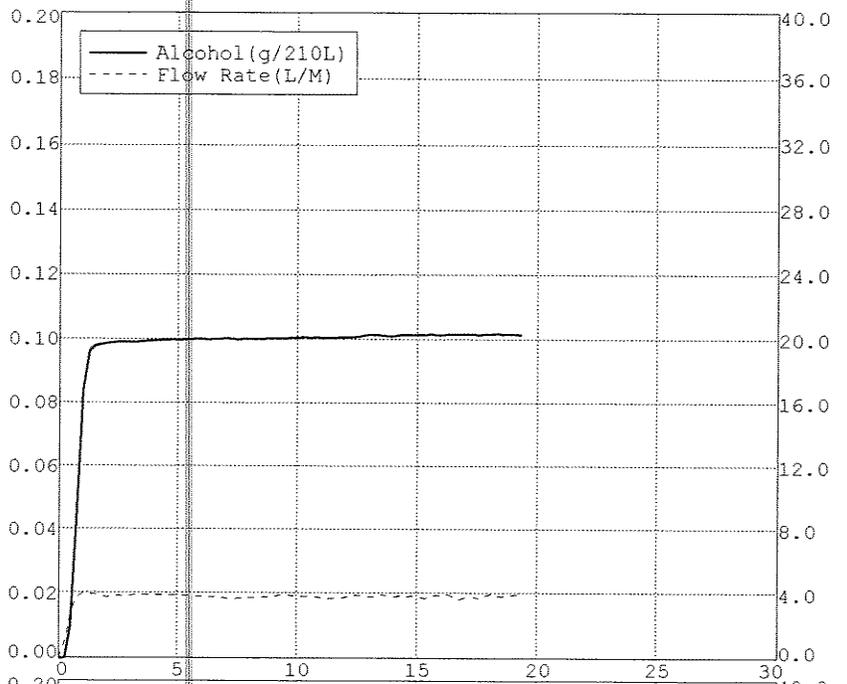

*Handwritten signature: Charles B. Geisler #201*