

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 11/02/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	13:58
INTERNAL STANDARD	VERIFIED	13:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:58
BLANK TEST	0.00	13:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	13:59
BLANK TEST	0.00	14:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:00
BLANK TEST	0.00	14:01

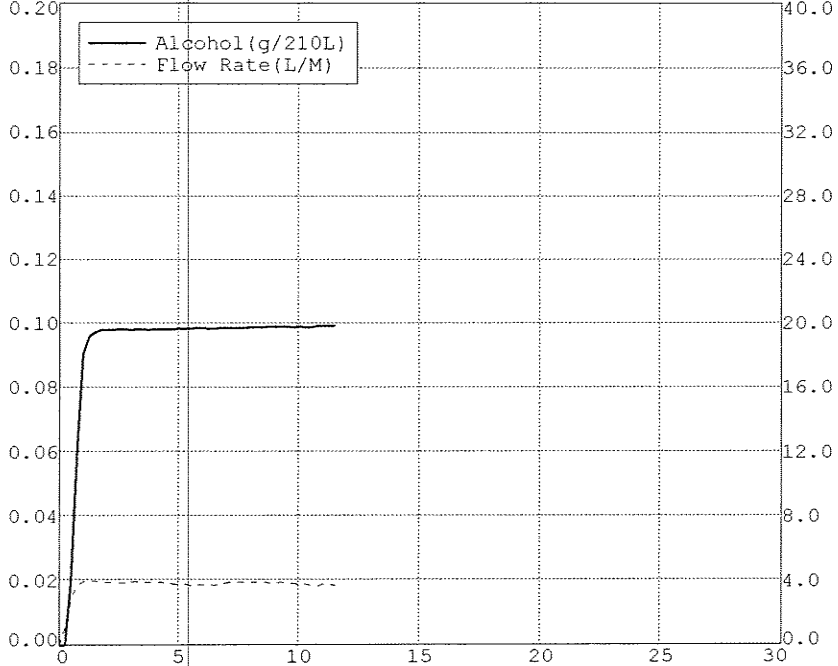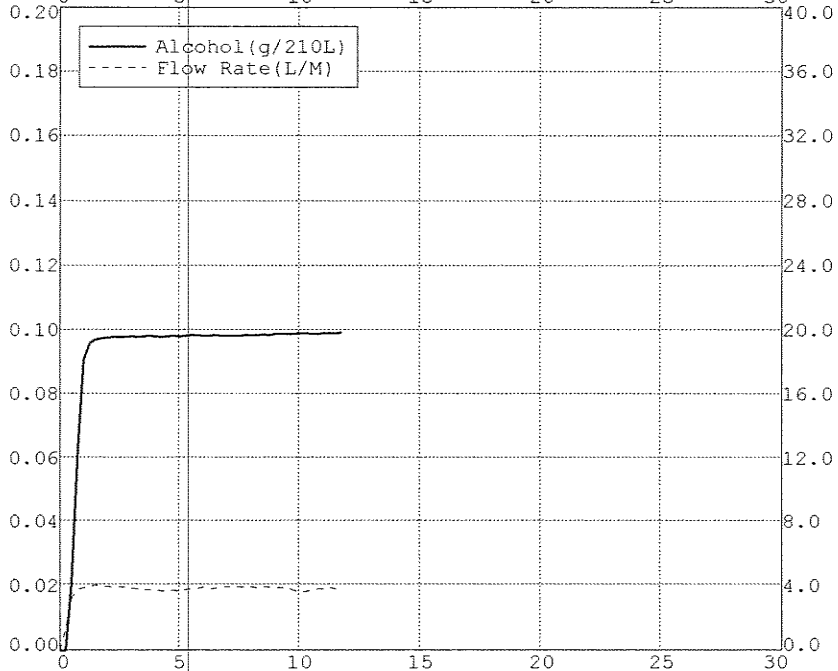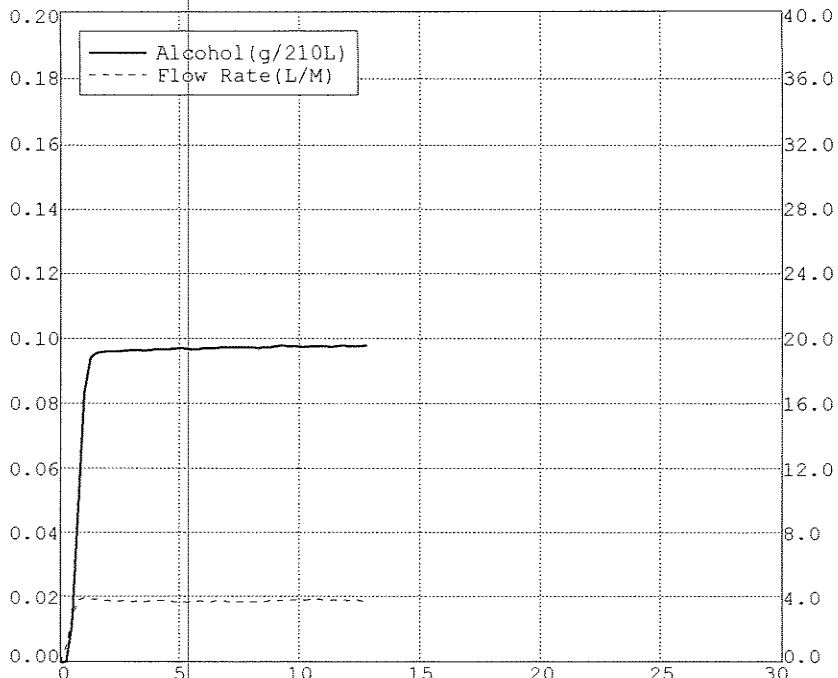

Charles B. Geisler #241