

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 11/25/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:02
INTERNAL STANDARD	VERIFIED	16:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:02
BLANK TEST	0.00	16:03
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:04
BLANK TEST	0.00	16:04
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:05
BLANK TEST	0.00	16:06

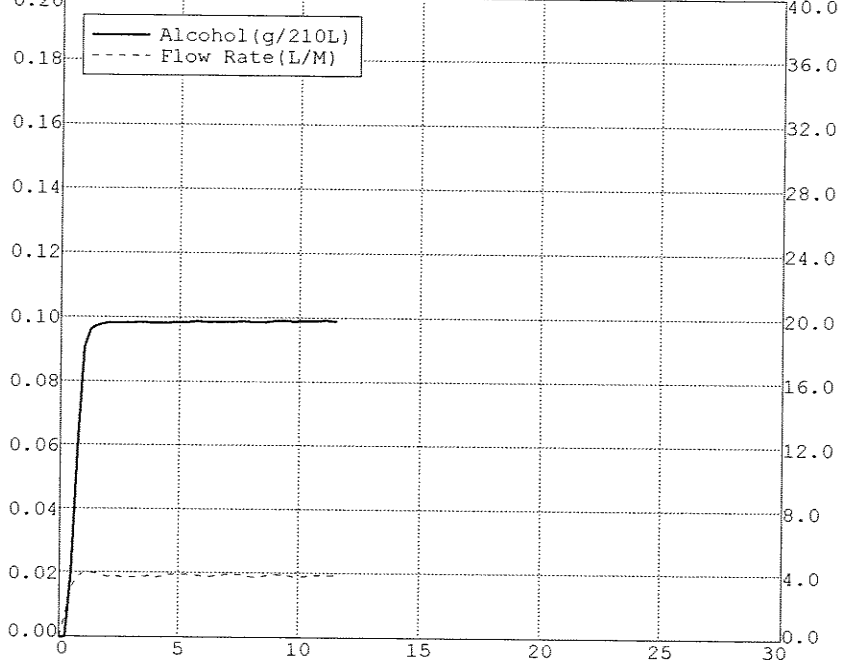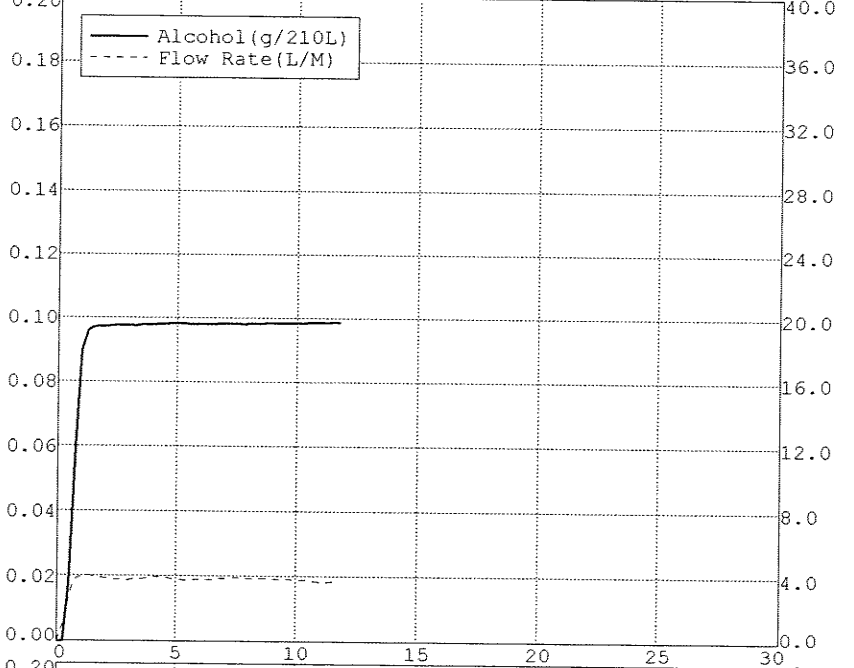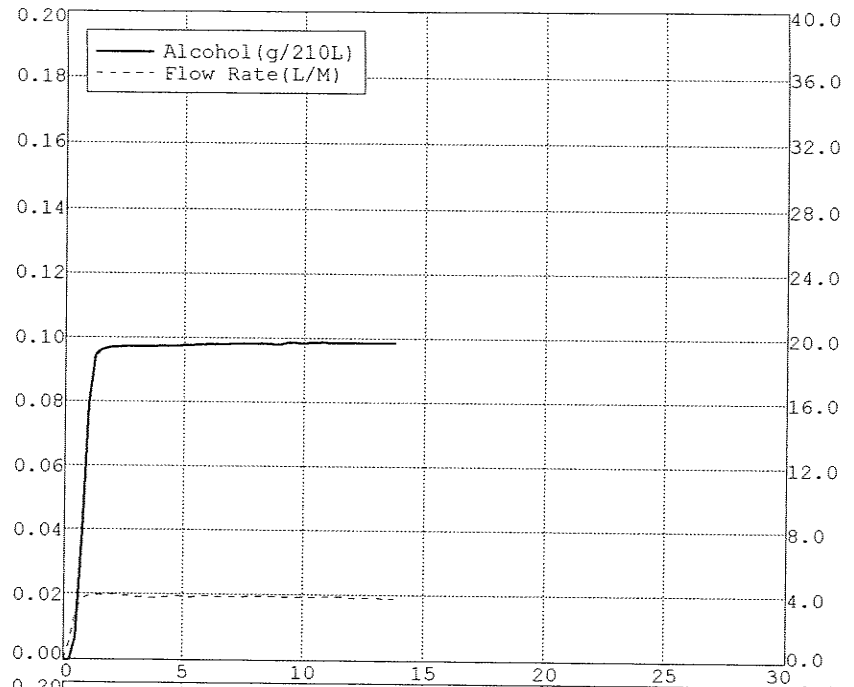

Charles B. Geisler
#241