

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 12/01/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:24
INTERNAL STANDARD	VERIFIED	17:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:25
BLANK TEST	0.00	17:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:26
BLANK TEST	0.00	17:27
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	17:27
BLANK TEST	0.00	17:28

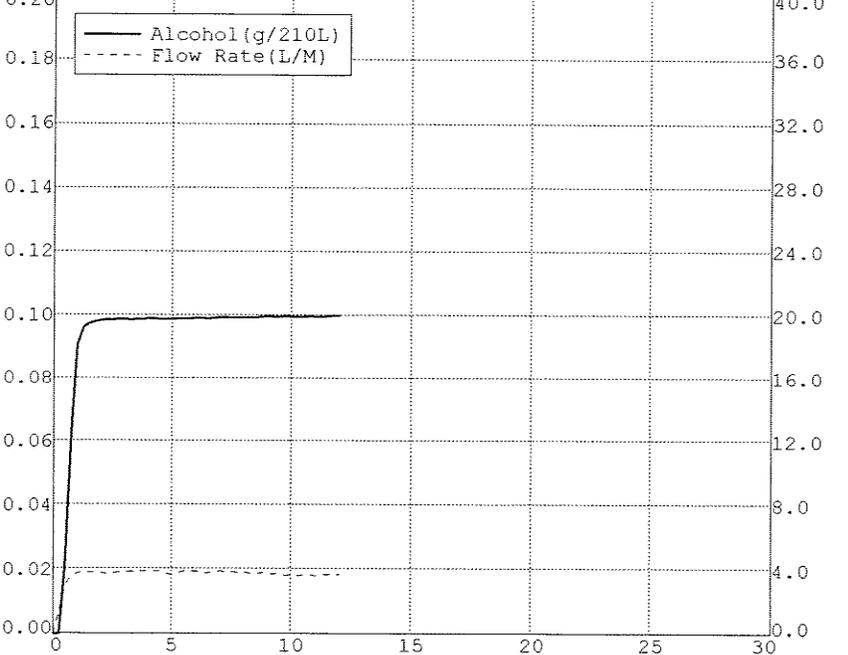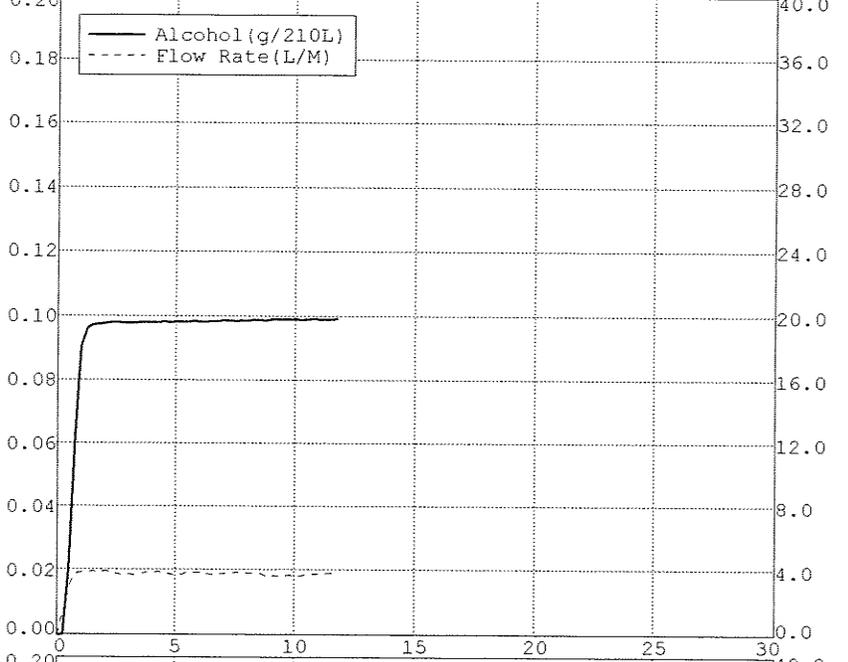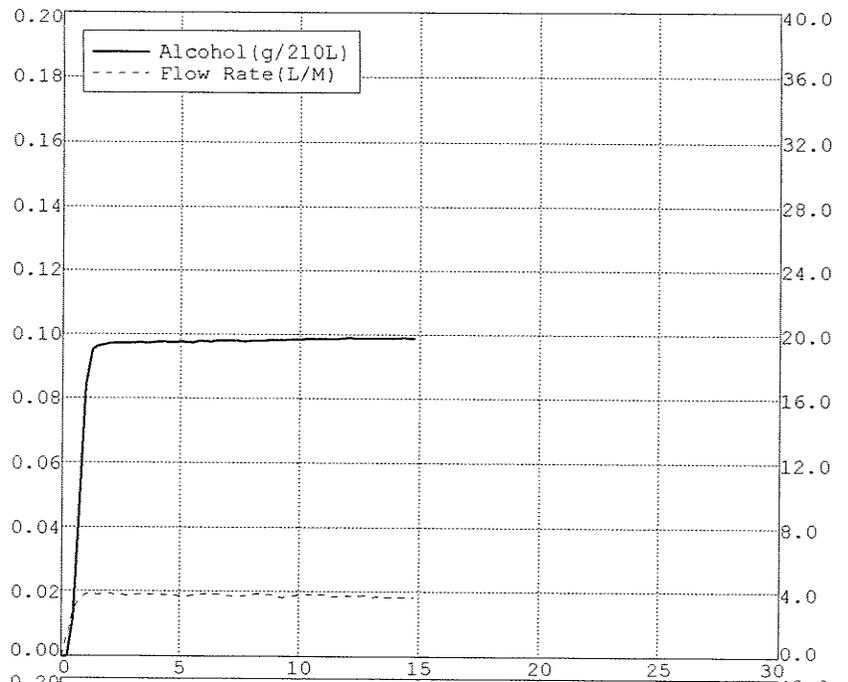

Charles B Geisler #218