

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 105208

Date: 12/20/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:34
INTERNAL STANDARD	VERIFIED	14:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:35
BLANK TEST	0.00	14:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:36
BLANK TEST	0.00	14:37
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:37
BLANK TEST	0.00	14:38

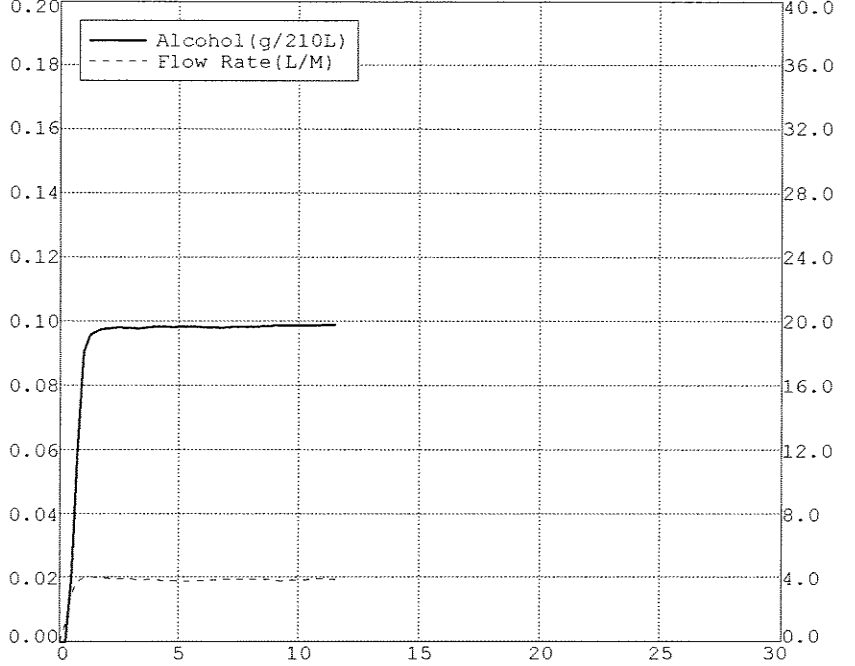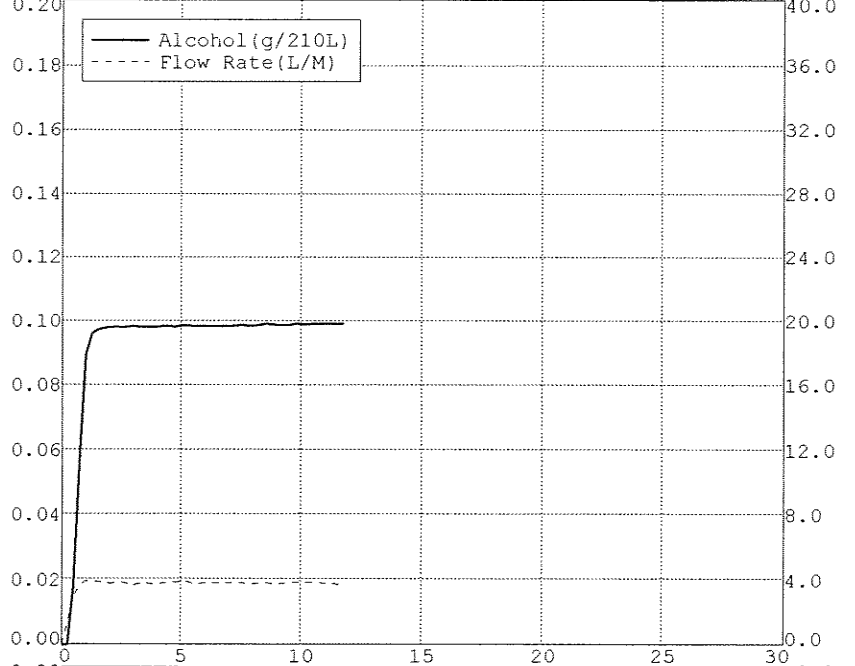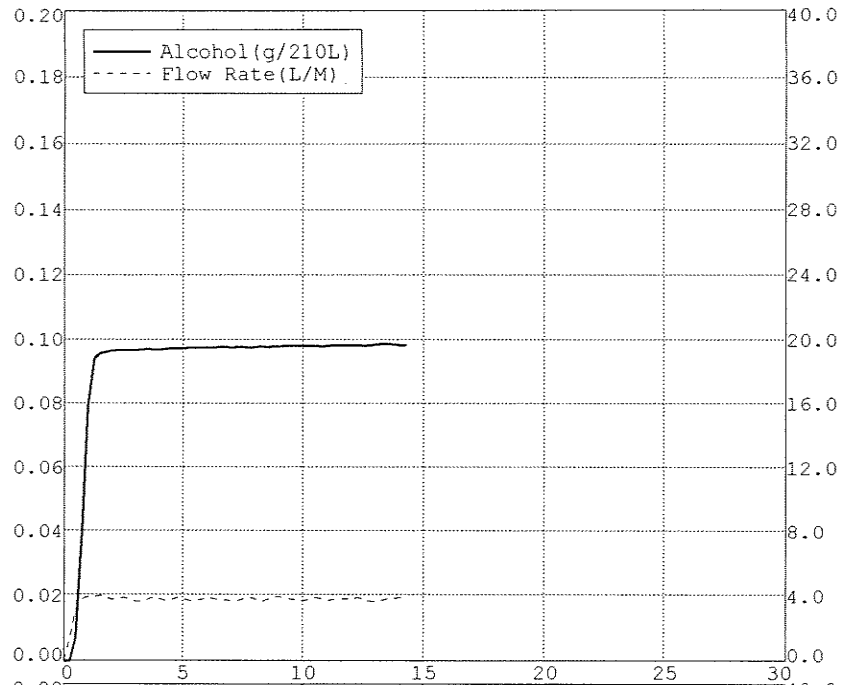

Sgt. Charles B. Geisler #245