

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 105208

Date: 12/28/2020

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 20430

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:12
INTERNAL STANDARD	VERIFIED	15:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:13
BLANK TEST	0.00	15:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:14
BLANK TEST	0.00	15:15
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:15
BLANK TEST	0.00	15:16

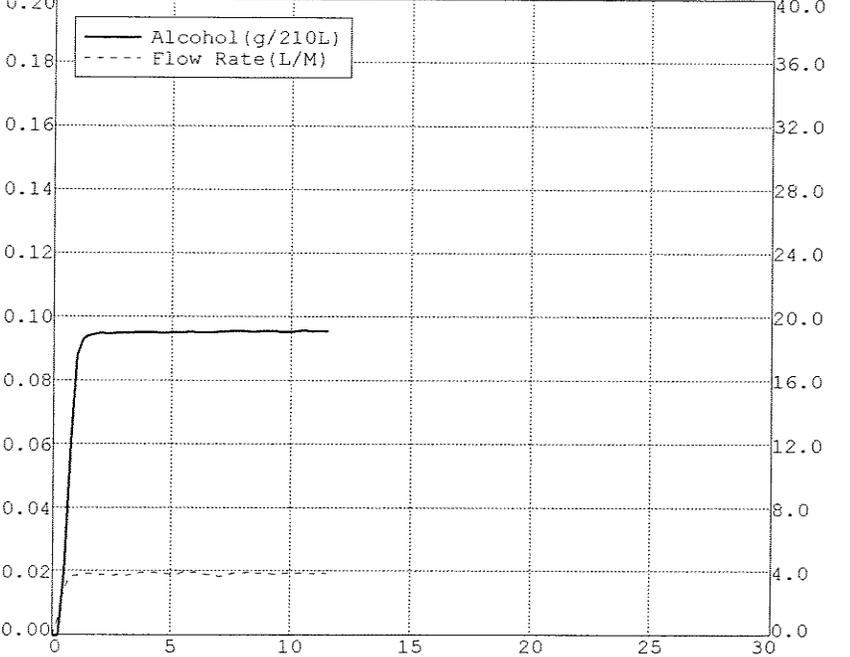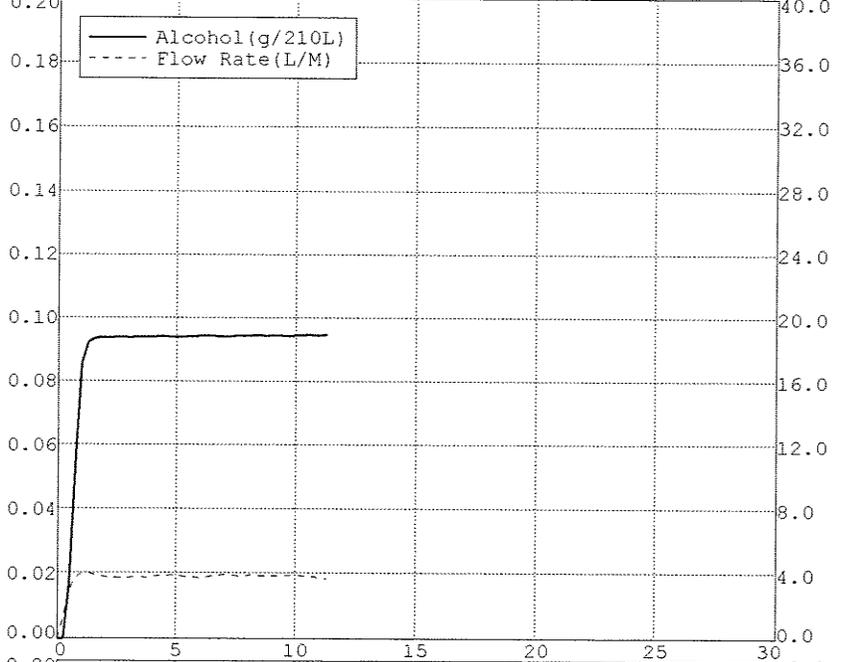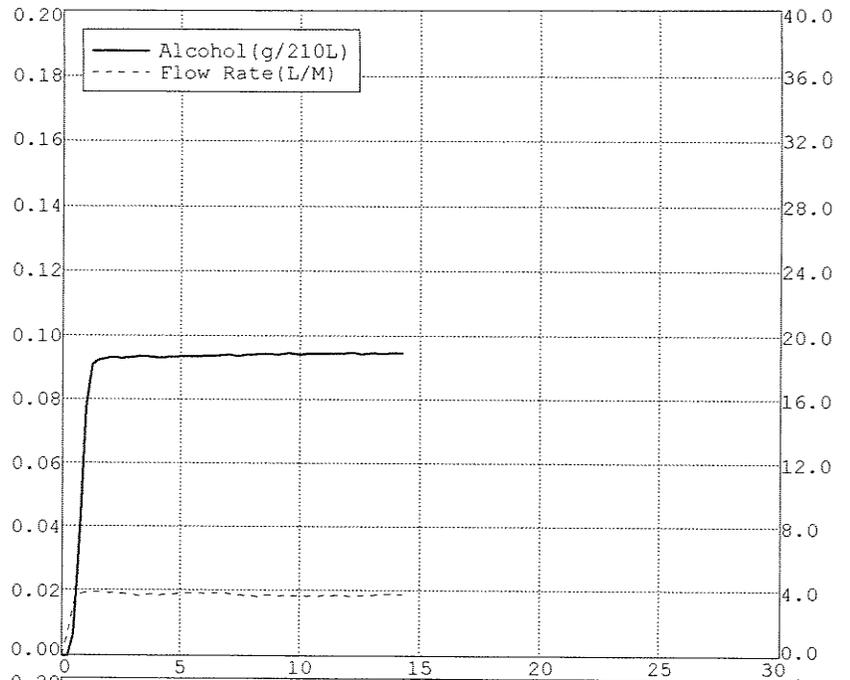

*Handwritten signature and initials*  
#211