

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 01/01/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	19:11
INTERNAL STANDARD	VERIFIED	19:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:11
BLANK TEST	0.00	19:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:12
BLANK TEST	0.00	19:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	19:14
BLANK TEST	0.00	19:15

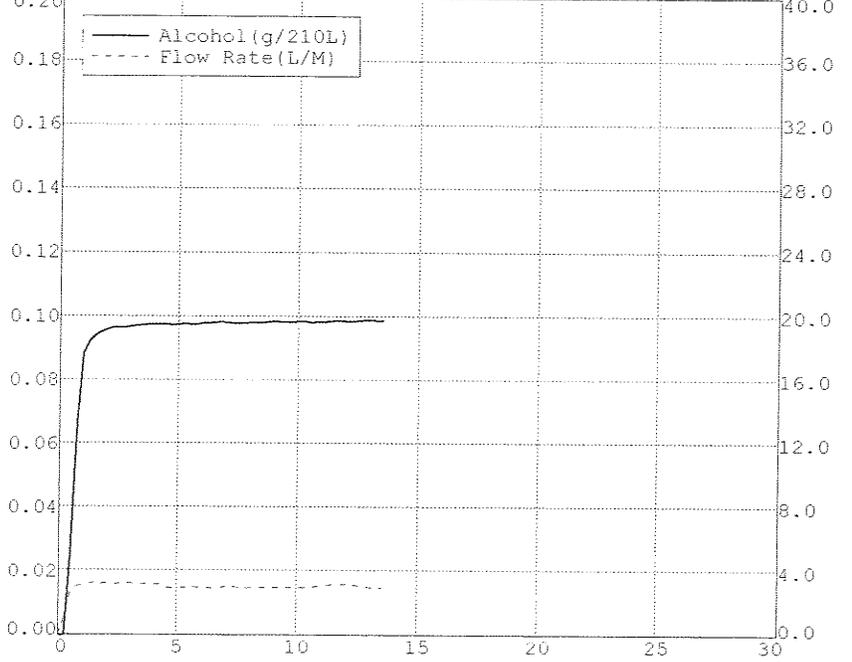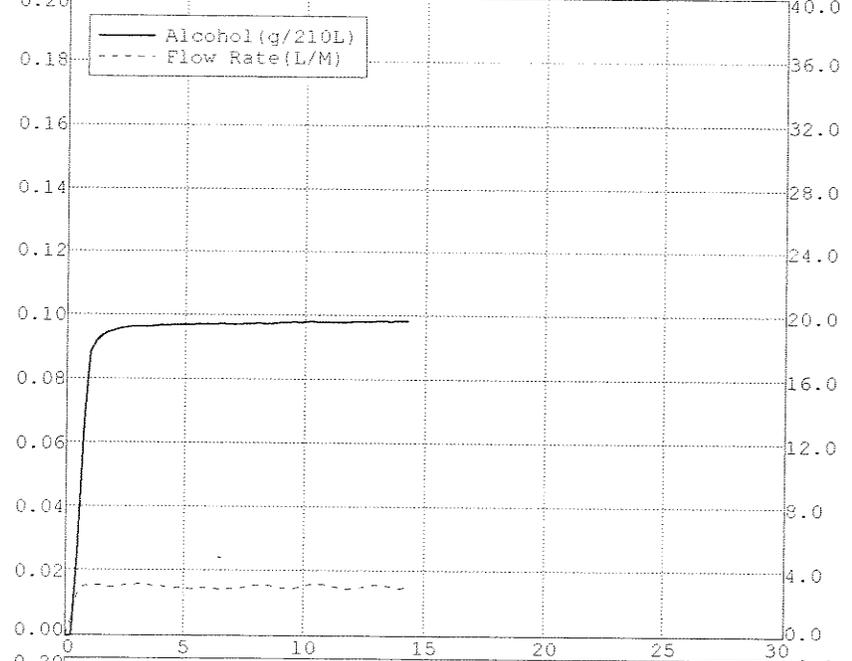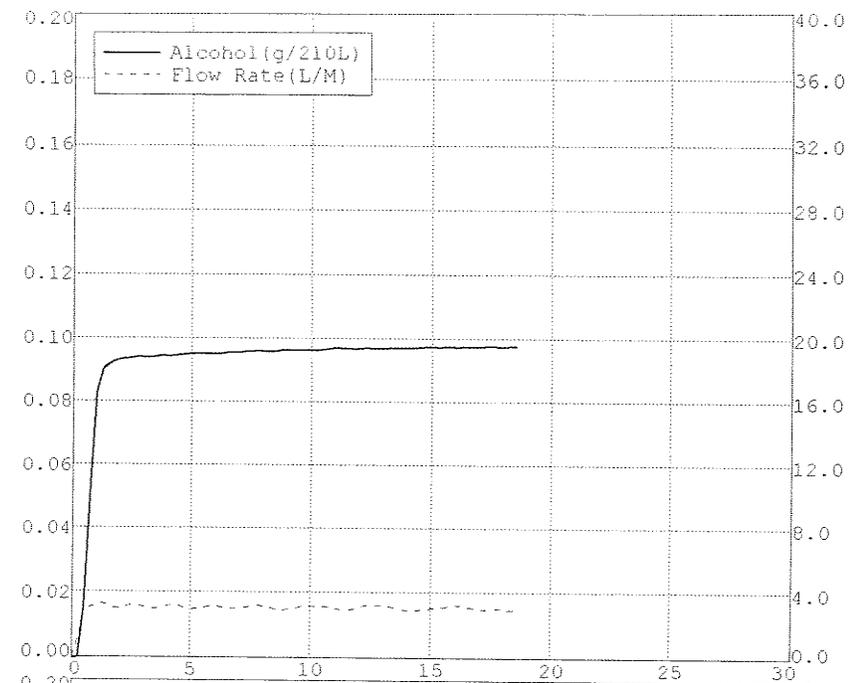

Charles B. Geisler #241