

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 01/13/2020

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	02:01
INTERNAL STANDARD	VERIFIED	02:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:02
BLANK TEST	0.00	02:03
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:03
BLANK TEST	0.00	02:04
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	02:04
BLANK TEST	0.00	02:05

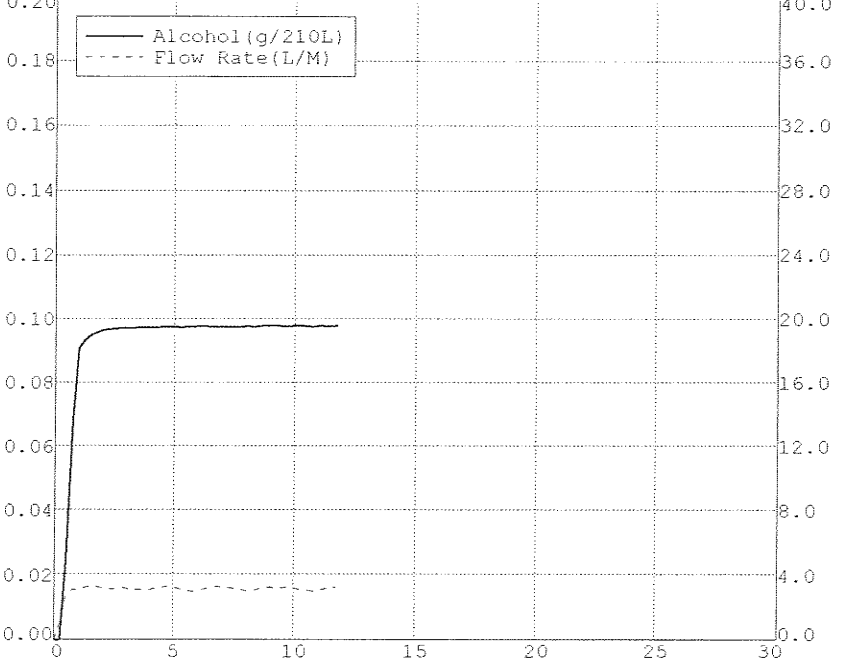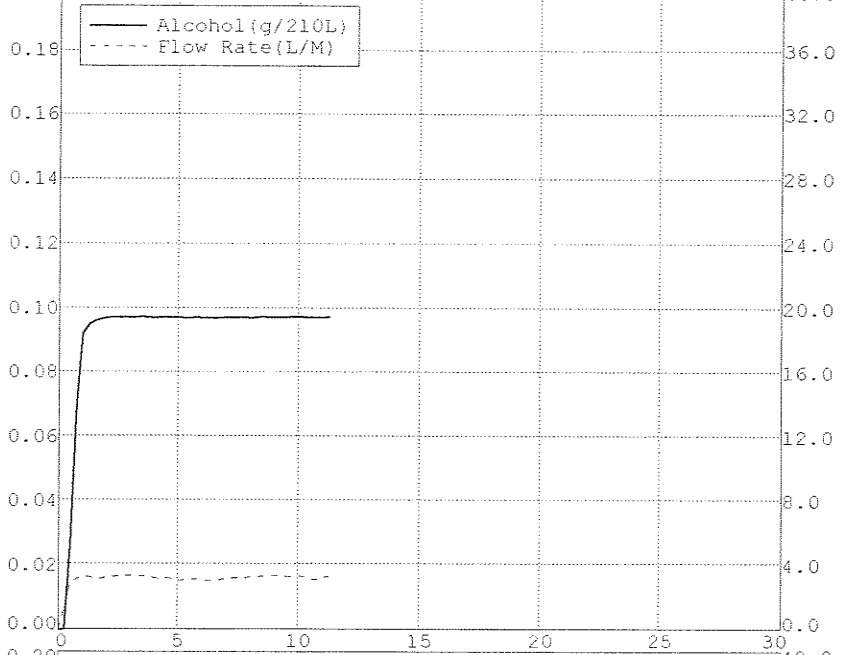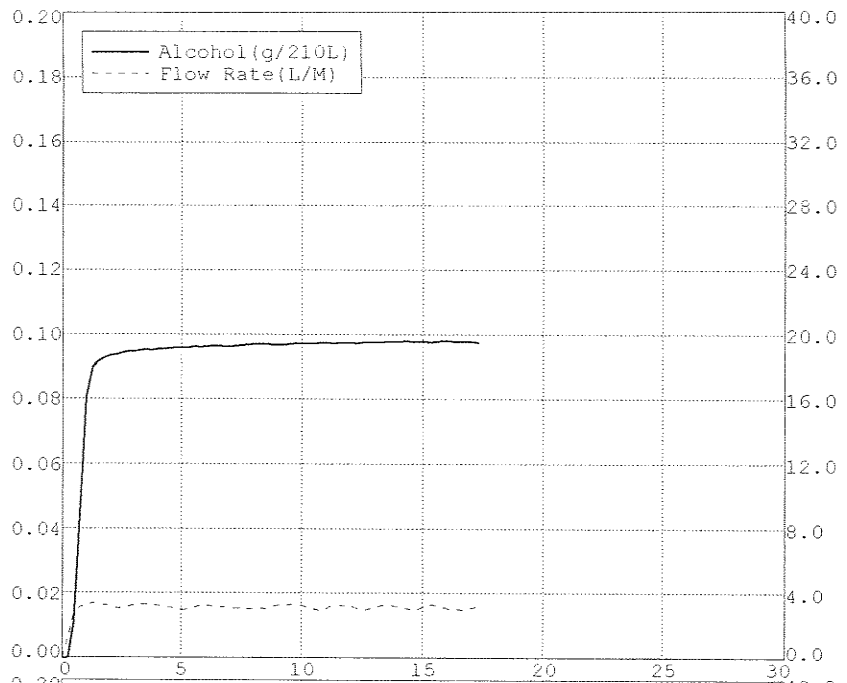

Sgt. M-B. [Signature] #24V