

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 01/27/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19250

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:59
INTERNAL STANDARD	VERIFIED	11:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:59
BLANK TEST	0.00	12:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:01
BLANK TEST	0.00	12:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:02
BLANK TEST	0.00	12:03

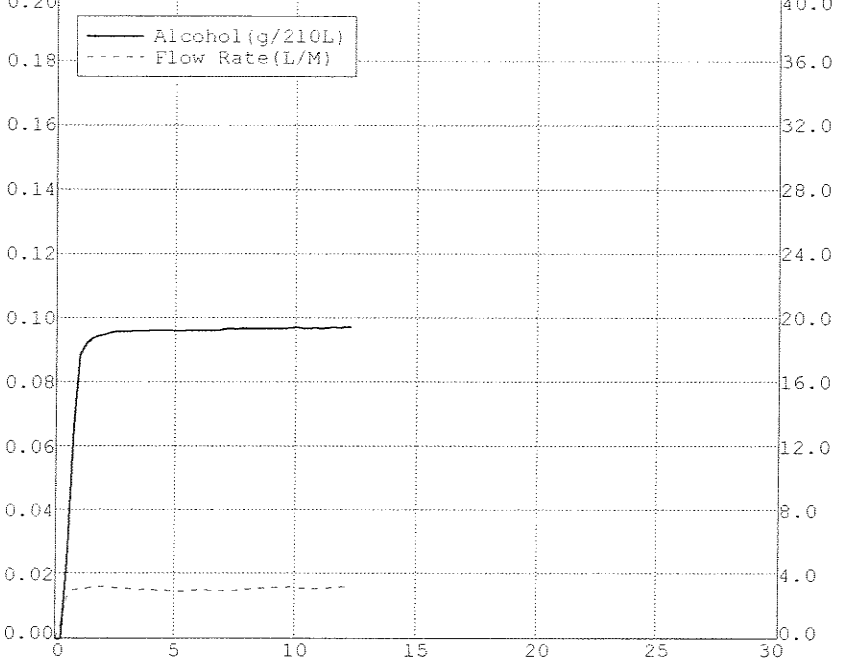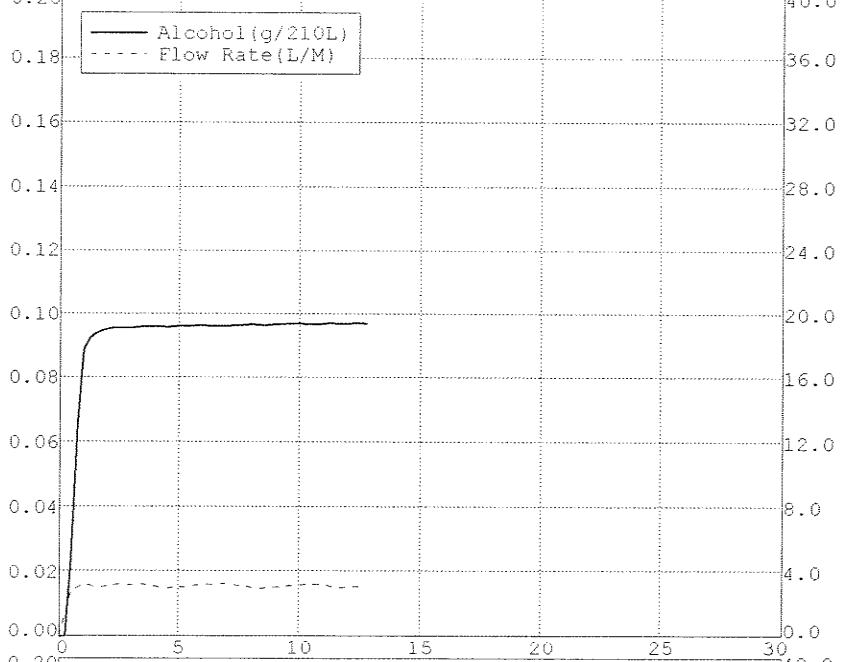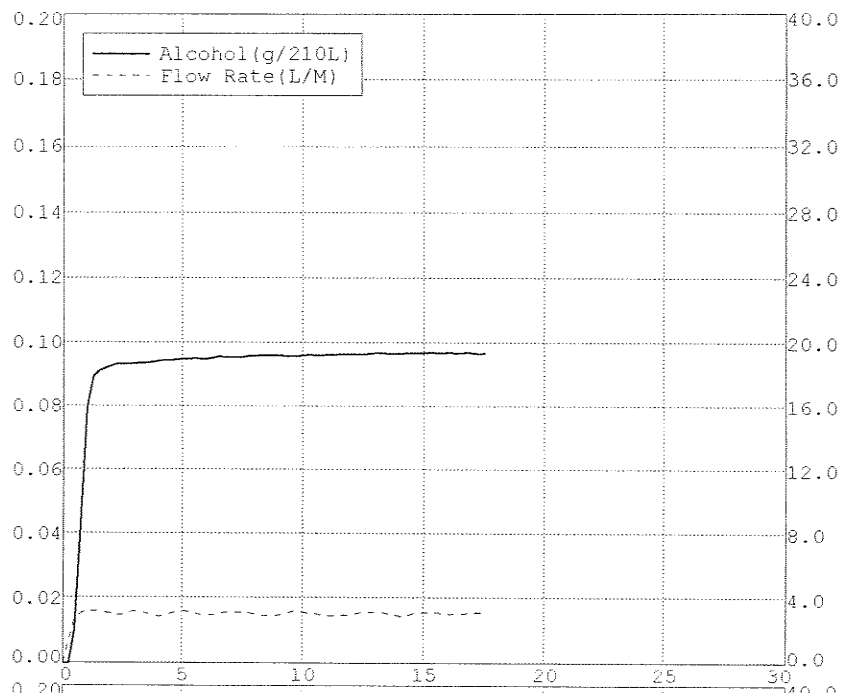

Charles B. Geisler #241