

SOLUTION CHANGE




-----  
 WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 106606  
 -----

Date: 02/01/2020

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:34
INTERNAL STANDARD	VERIFIED	10:34
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:34
BLANK TEST	0.00	10:35
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:36
BLANK TEST	0.00	10:36
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:37
BLANK TEST	0.00	10:38

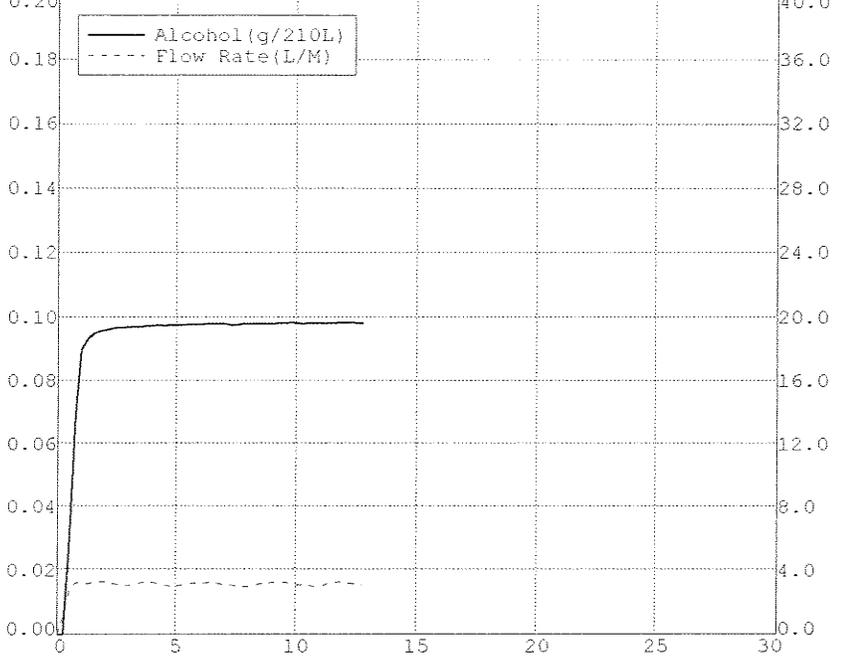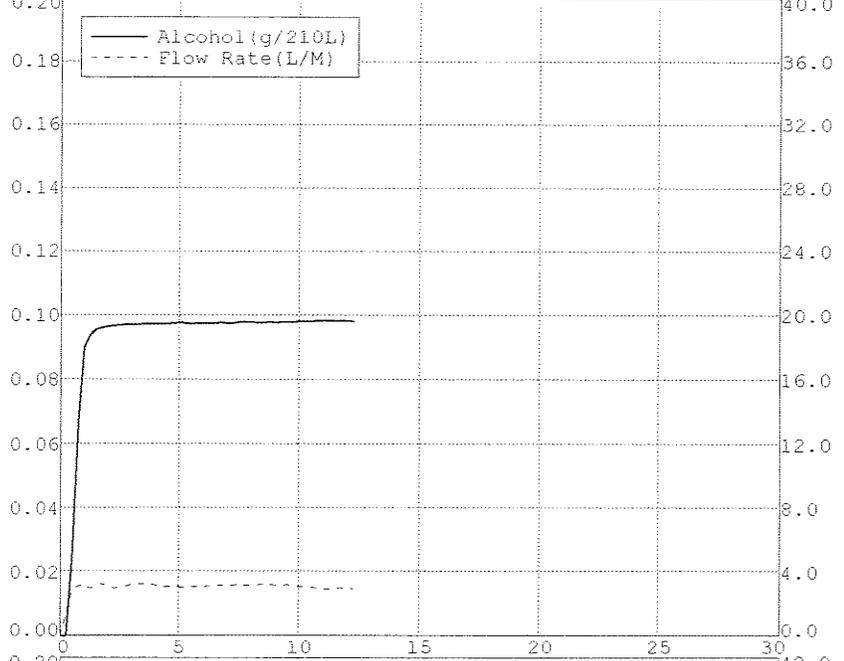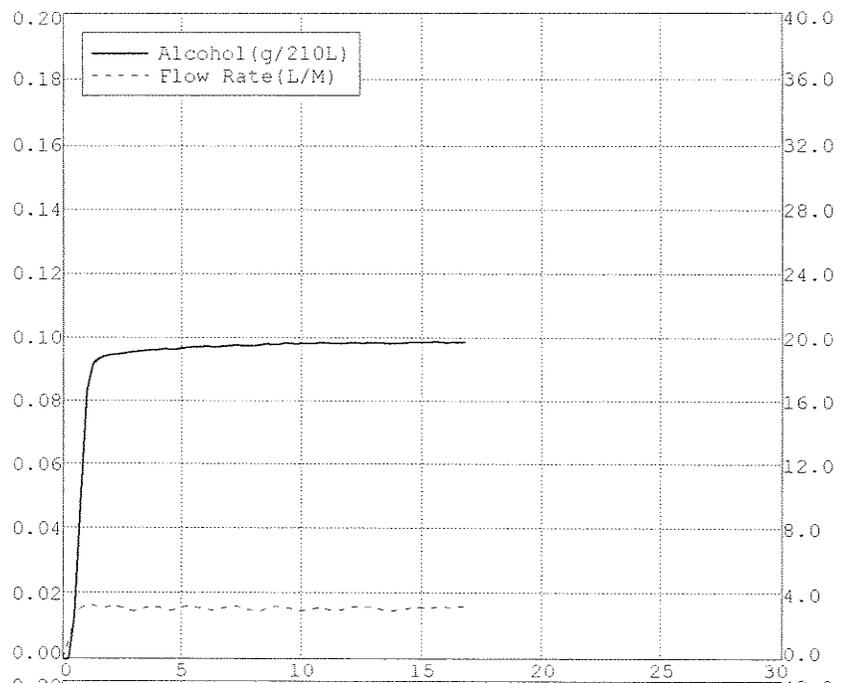

*Sgt. C. B. Geisler #244*