

SUPERVISOR TEST



WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 02/06/2020

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:59
INTERNAL STANDARD	VERIFIED	14:59
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:00
BLANK TEST	0.00	15:01
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:01
BLANK TEST	0.00	15:02
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:02
BLANK TEST	0.00	15:03

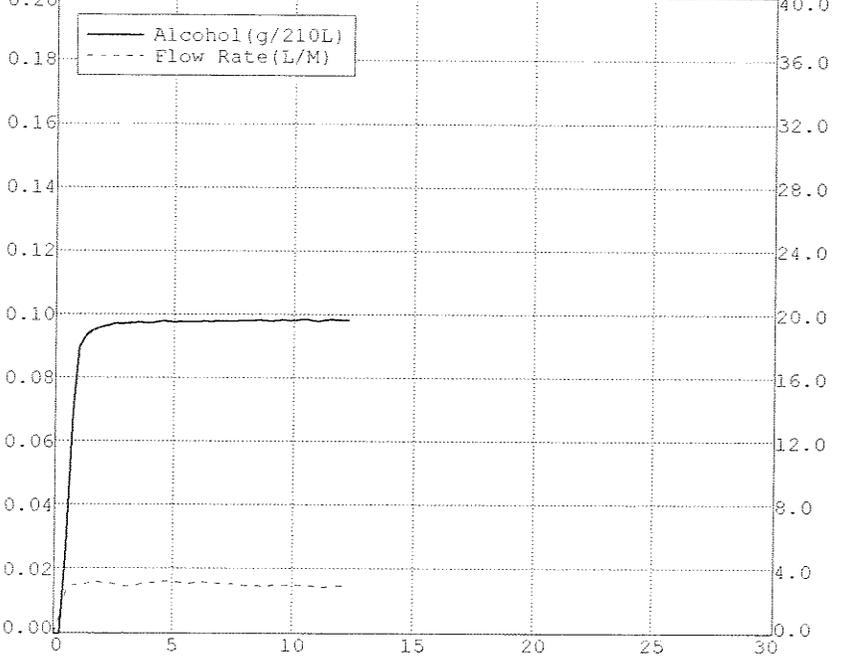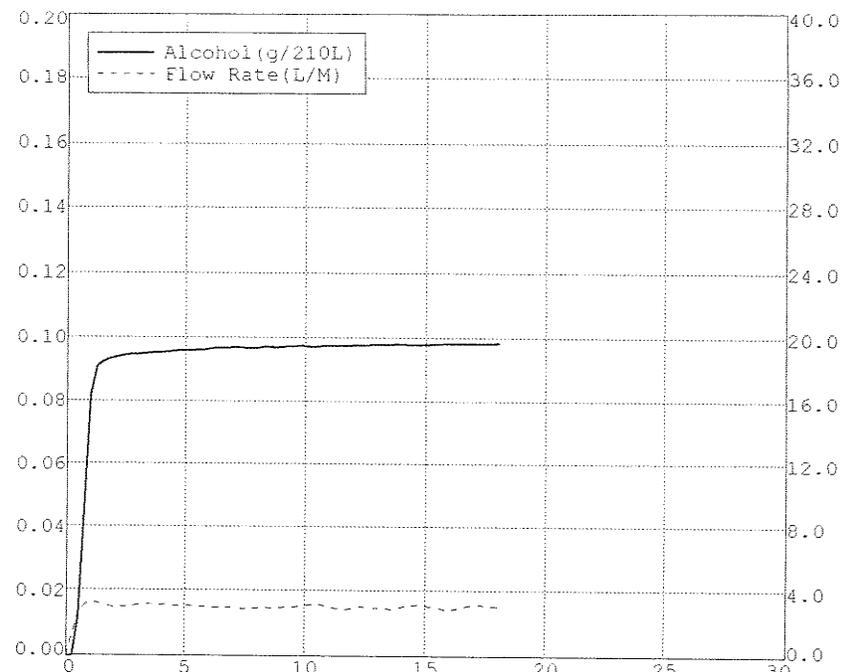

*Sgt. Charles B. Geisler* #245