

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 02/19/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	16:56
INTERNAL STANDARD	VERIFIED	16:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:57
BLANK TEST	0.00	16:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	16:58
BLANK TEST	0.00	16:59
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.09	16:59
BLANK TEST	0.00	17:00

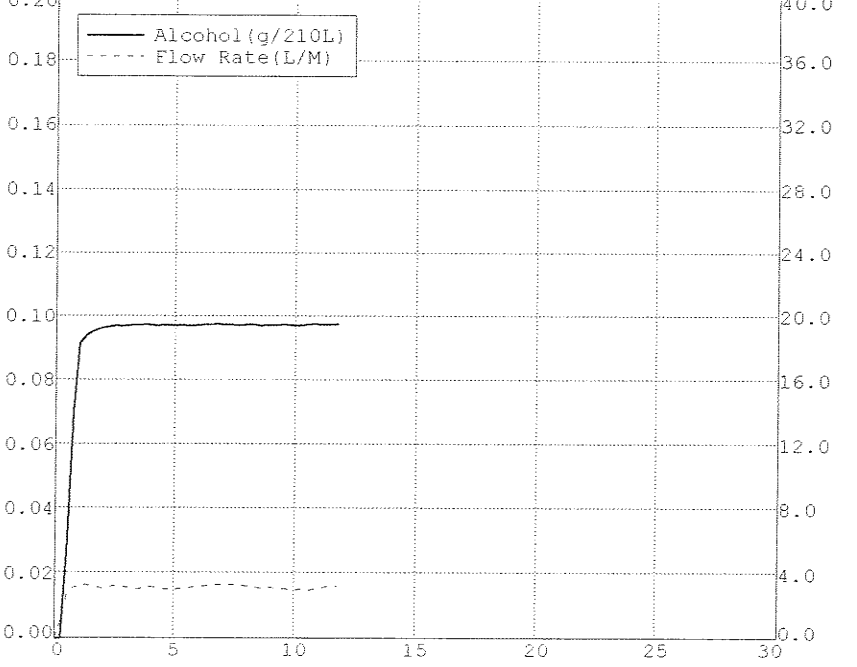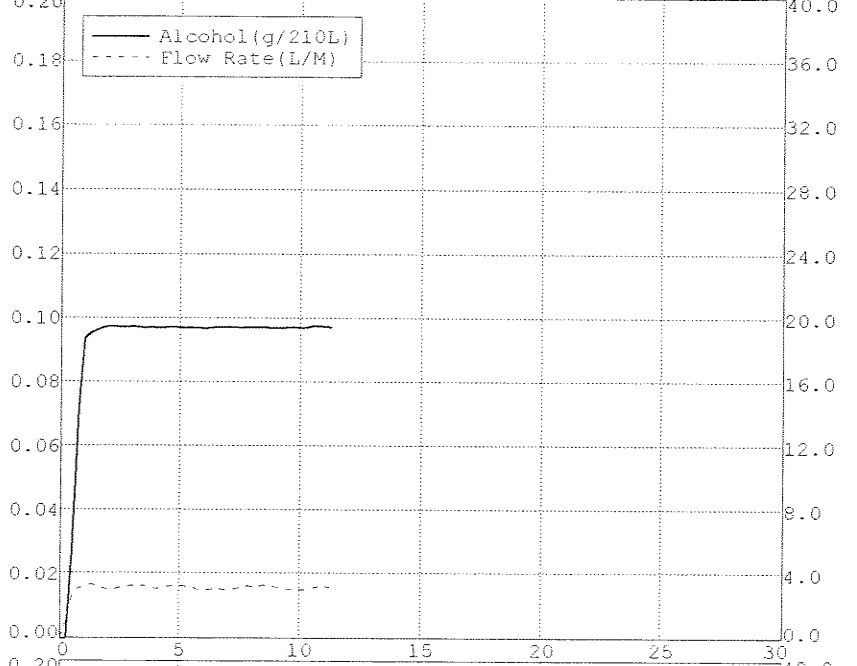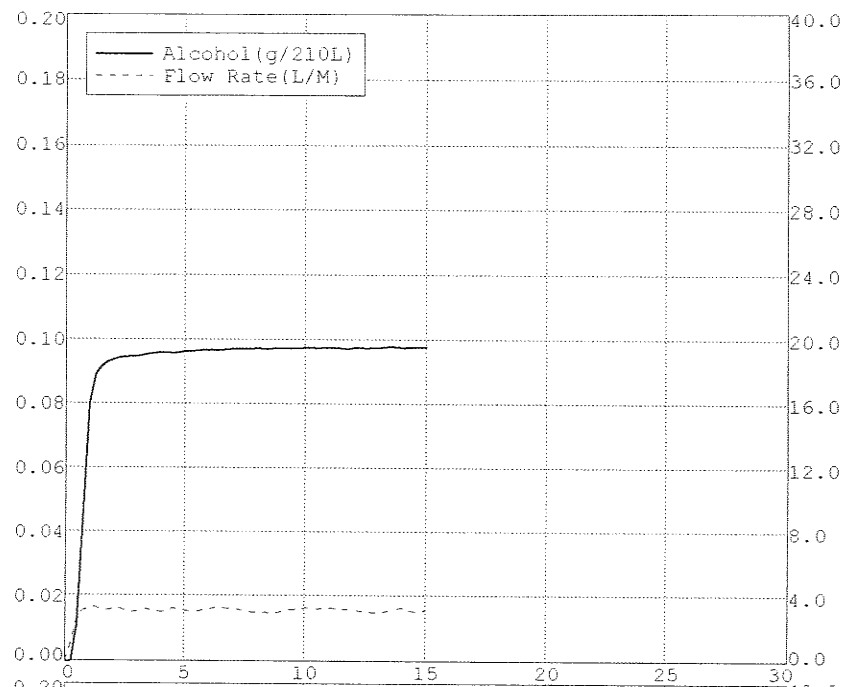

Handwritten signatures and initials.