

SUPERVISOR TEST




WARREN CO.
 SHERIFF'S OFFICE
 DATAMASTER dmt: 106606

Date: 03/09/2020

OPERATOR NAME:
 CHARLES B GEISLER
 Permit #: 33757
 Operator Agency/Dept: WARREN CO. SO
 Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	11:06
INTERNAL STANDARD	VERIFIED	11:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:07
BLANK TEST	0.00	11:08
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:08
BLANK TEST	0.00	11:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	11:09
BLANK TEST	0.00	11:10

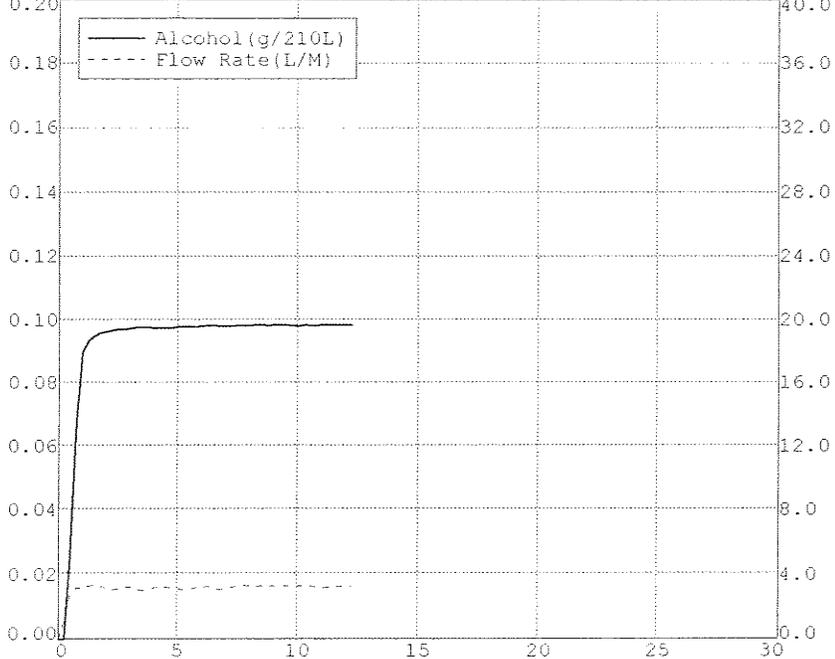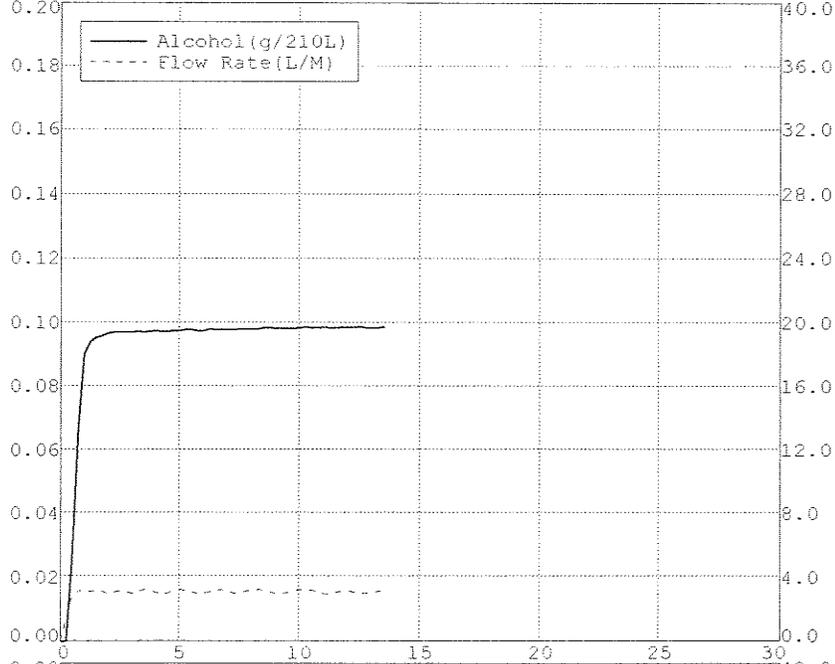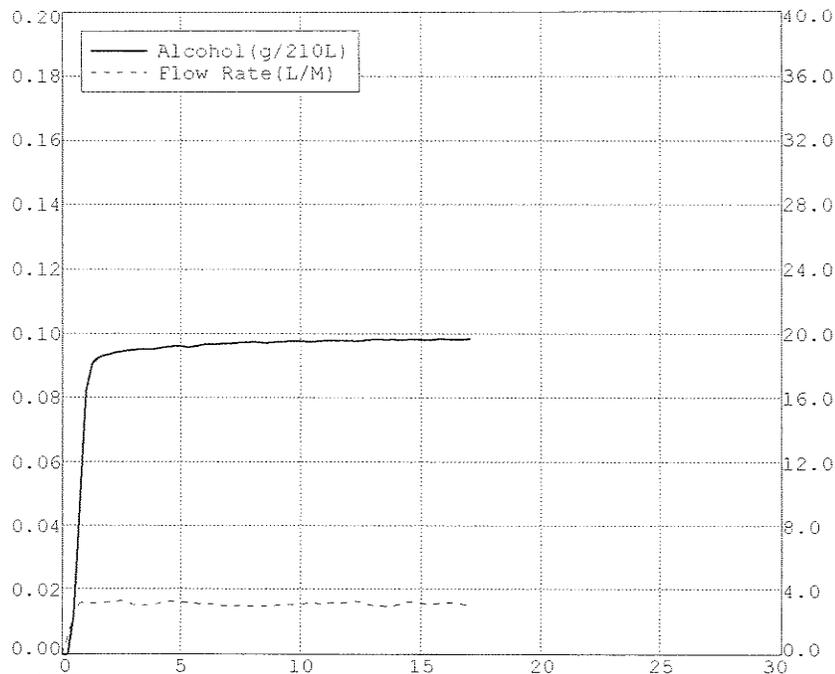

Signature: Charles B. Geisler #248