

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 03/23/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:58
INTERNAL STANDARD	VERIFIED	14:58
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	14:59
BLANK TEST	0.00	15:00
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:00
BLANK TEST	0.00	15:01
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:01
BLANK TEST	0.00	15:02

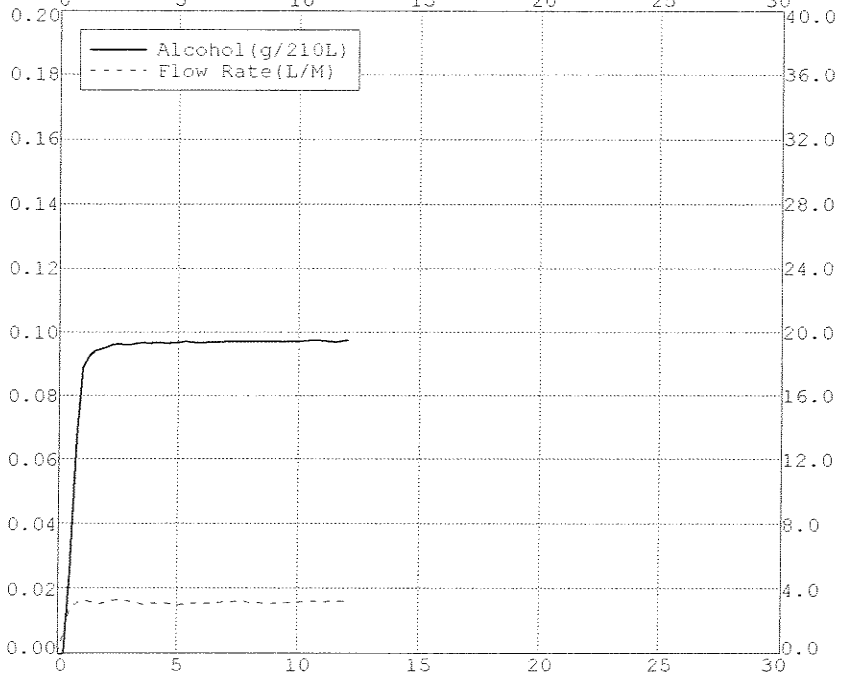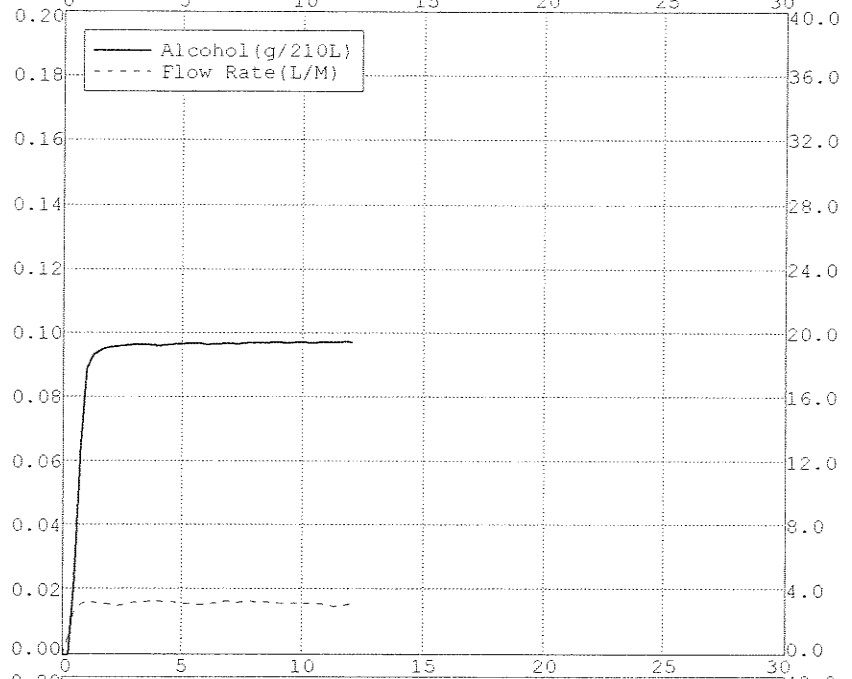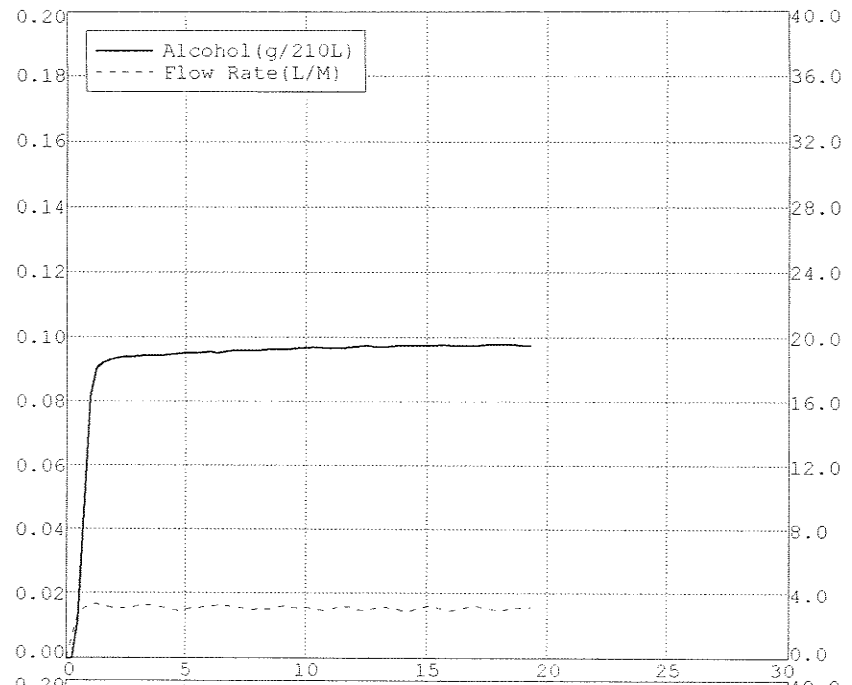

Sgt. C. B. Geisler #248