

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 03/29/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 19350

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:09
INTERNAL STANDARD	VERIFIED	15:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:09
BLANK TEST	0.00	15:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:10
BLANK TEST	0.00	15:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:12
BLANK TEST	0.00	15:13

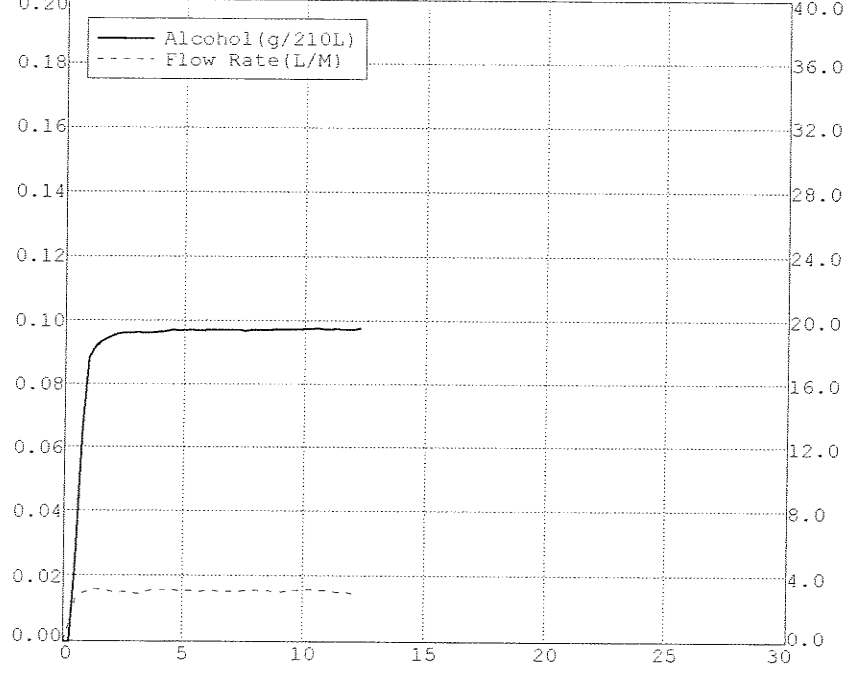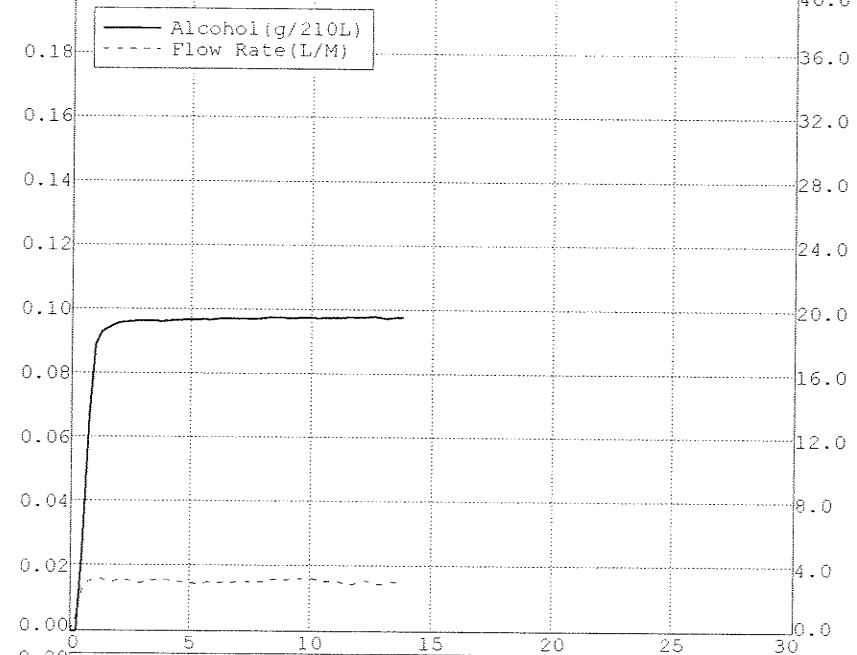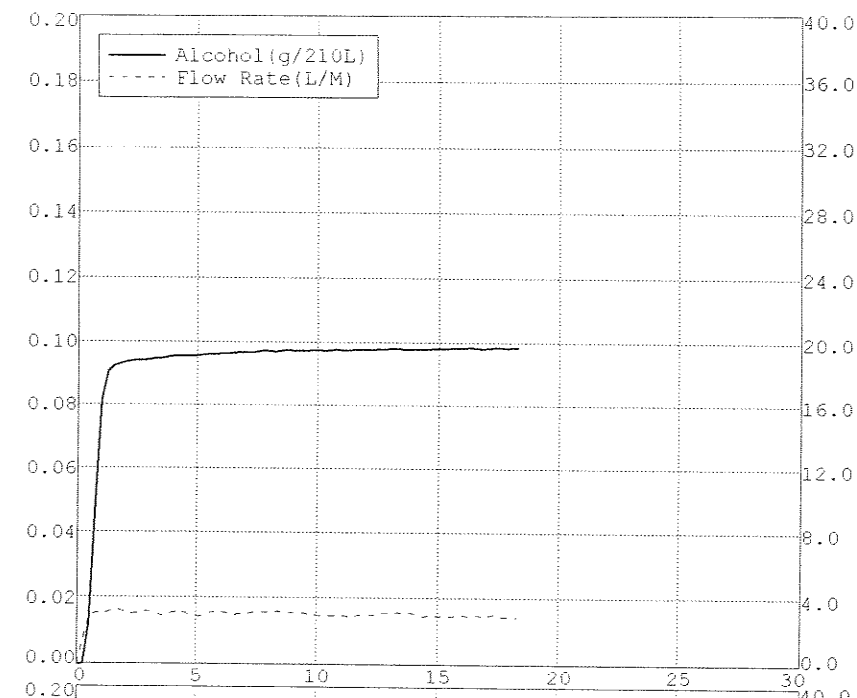

Charles B. Geisler