

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 04/01/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:31
INTERNAL STANDARD	VERIFIED	10:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:31
BLANK TEST	0.00	10:32
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:32
BLANK TEST	0.00	10:33
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:33
BLANK TEST	0.00	10:34

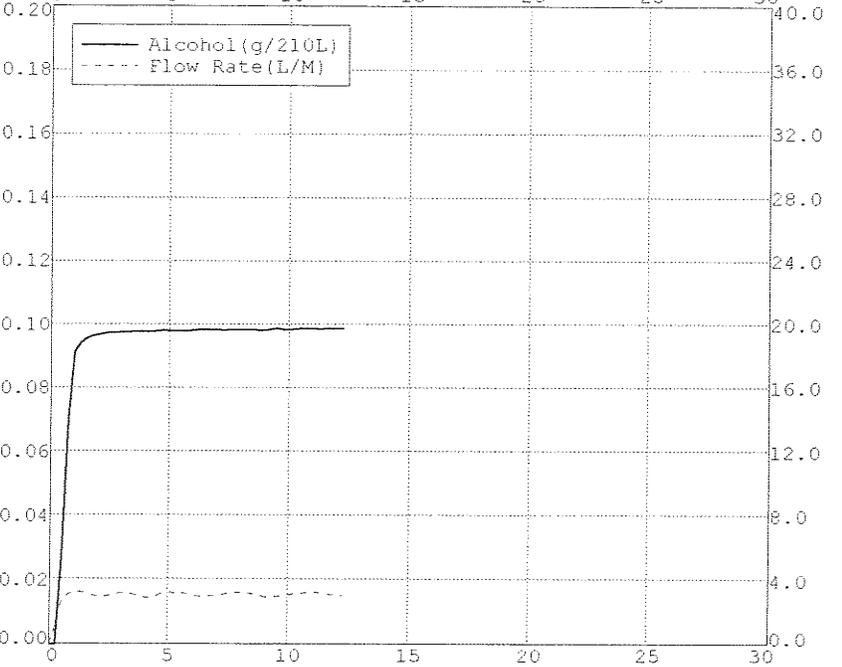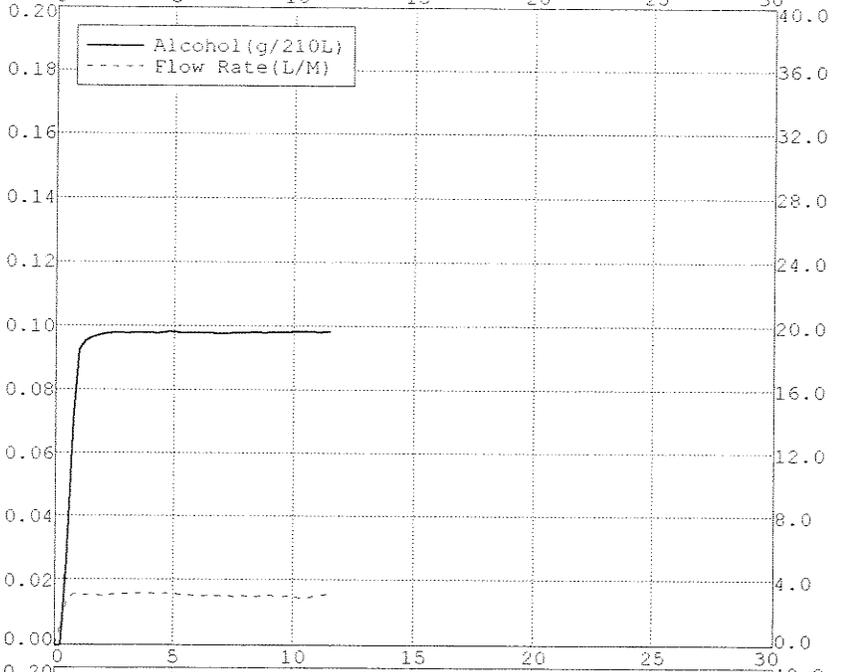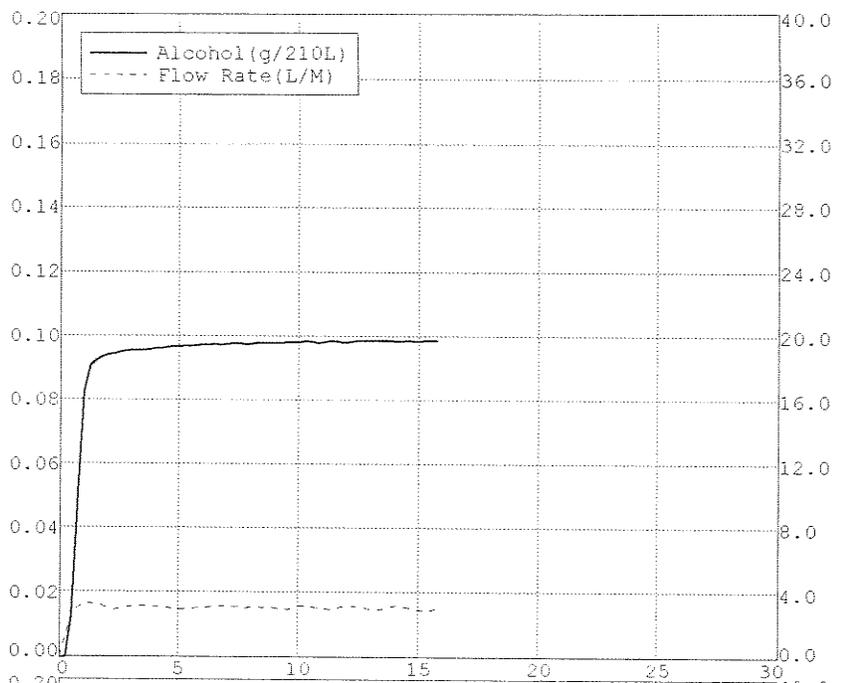

Sgt. Charles B. Geisler