

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 04/15/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:22
INTERNAL STANDARD	VERIFIED	17:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:22
BLANK TEST	0.00	17:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:23
BLANK TEST	0.00	17:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:25
BLANK TEST	0.00	17:25

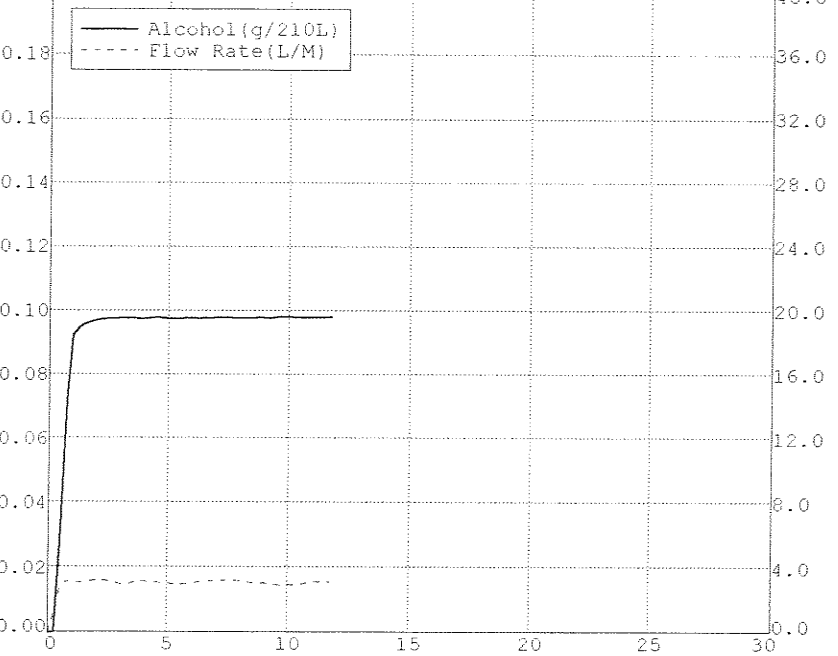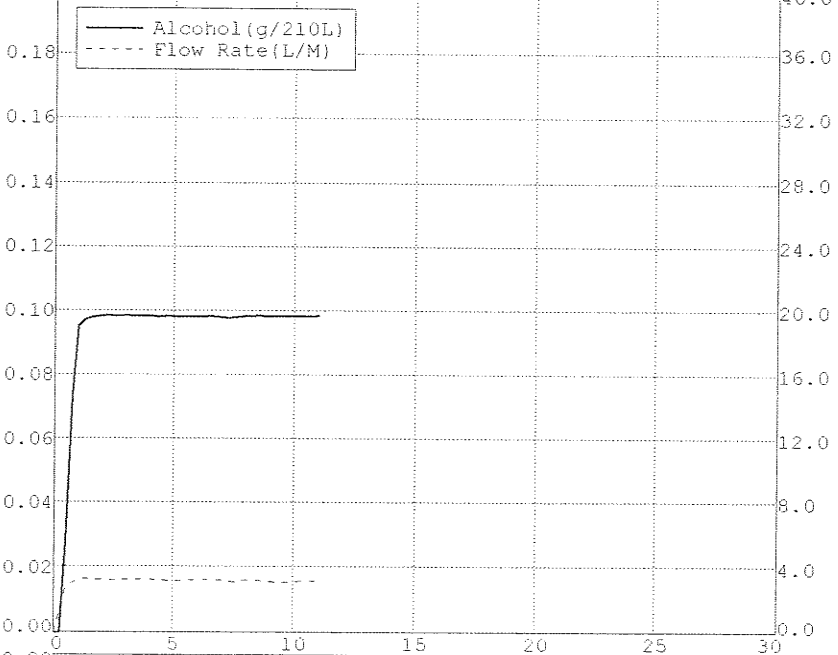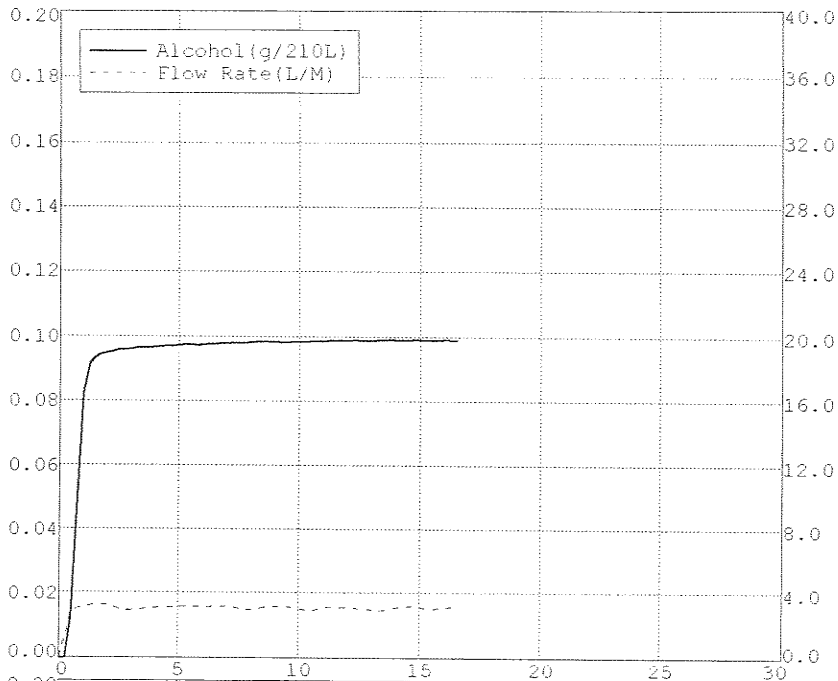

Ch. B. Geisler #244