

SOLUTION CHANGE




WARREN CO.  
 SHERIFF'S OFFICE  
 DATAMASTER dmt: 106606

Date: 04/30/2020

OPERATOR NAME:  
 CHARLES B GEISLER  
 Permit #: 33757  
 Operator Agency/Dept: WARREN CO. SO  
 Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:21
INTERNAL STANDARD	VERIFIED	09:21
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	09:21
BLANK TEST	0.00	09:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:22
BLANK TEST	0.00	09:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:24
BLANK TEST	0.00	09:25

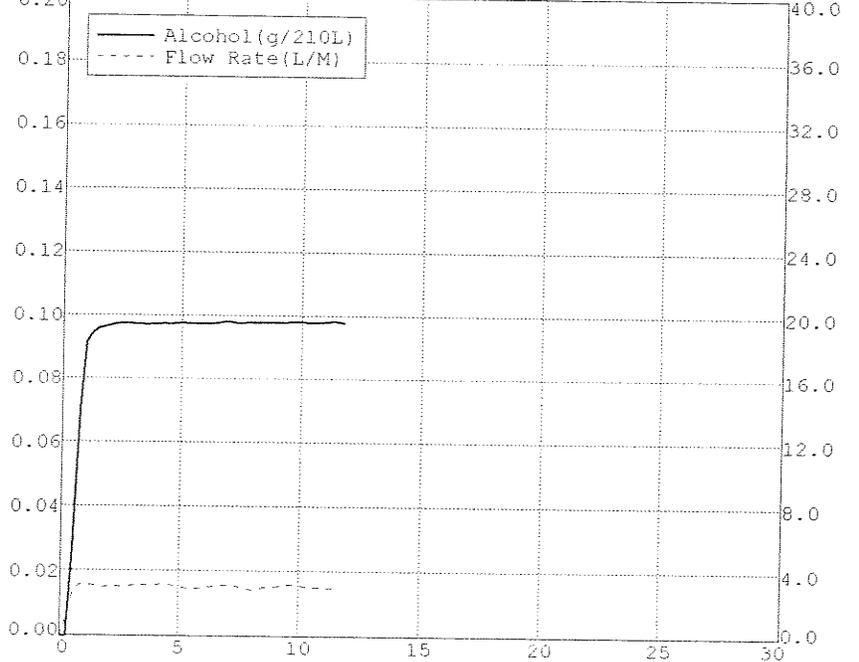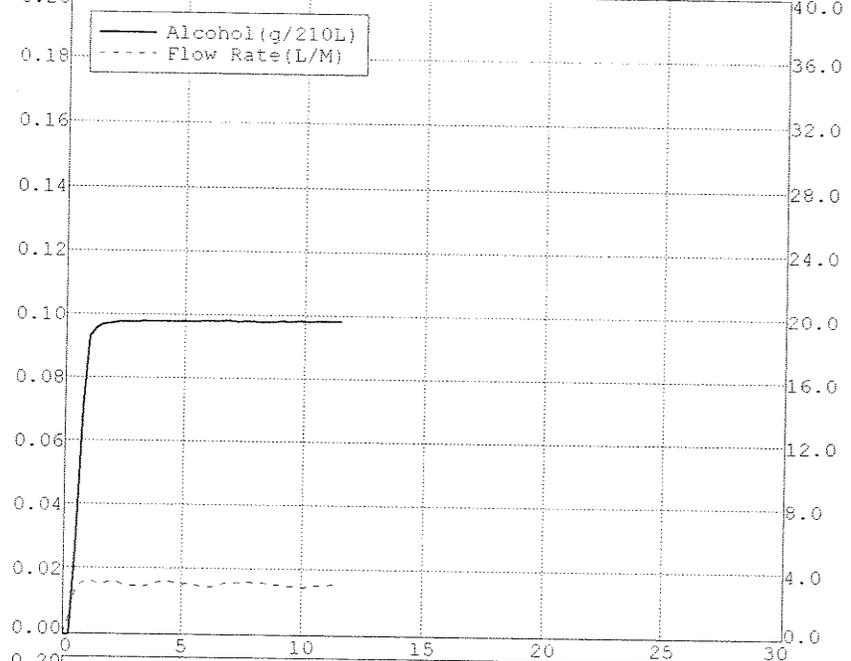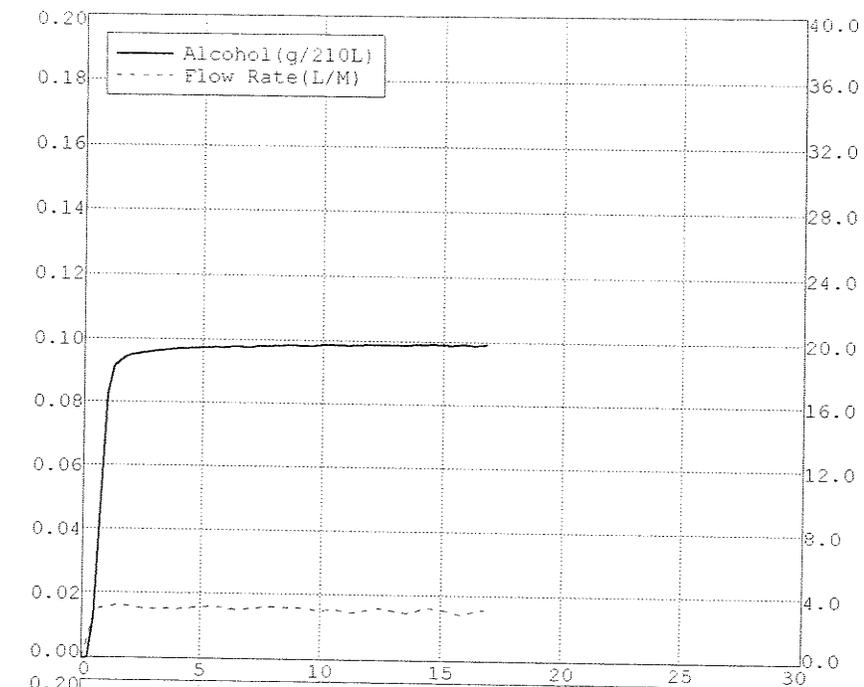

*Charles B. Geisler #244*