

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 05/19/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	12:05
INTERNAL STANDARD	VERIFIED	12:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:05
BLANK TEST	0.00	12:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:07
BLANK TEST	0.00	12:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	12:08
BLANK TEST	0.00	12:09

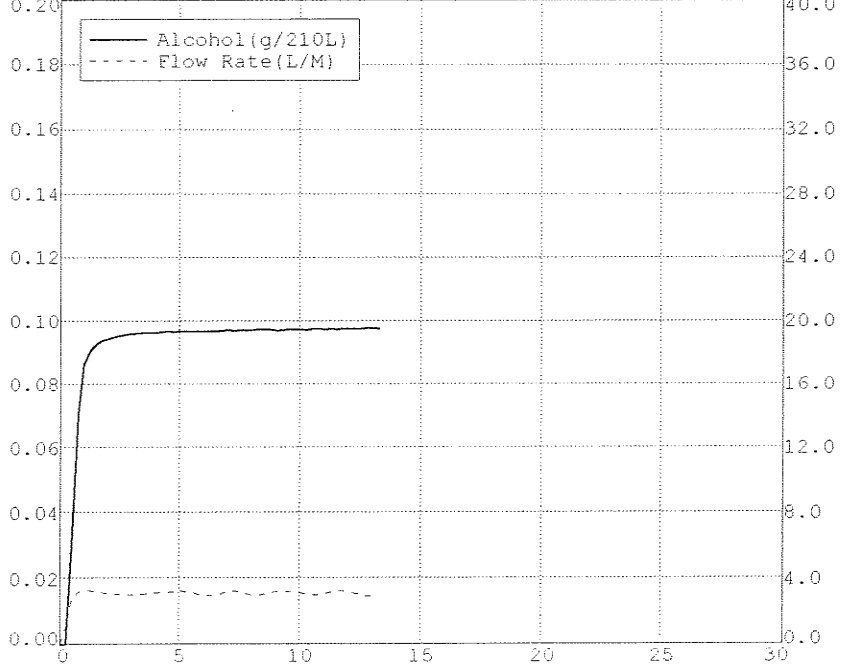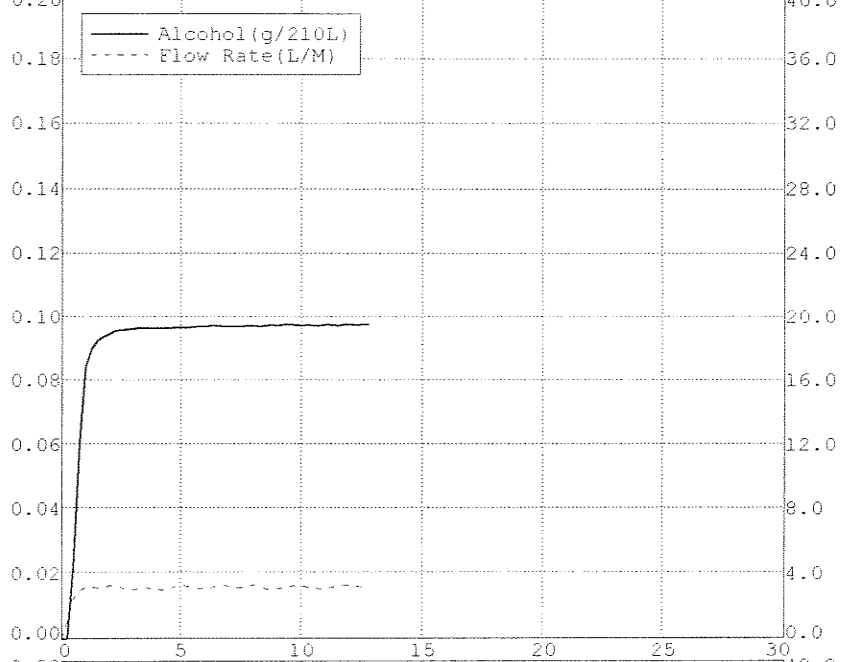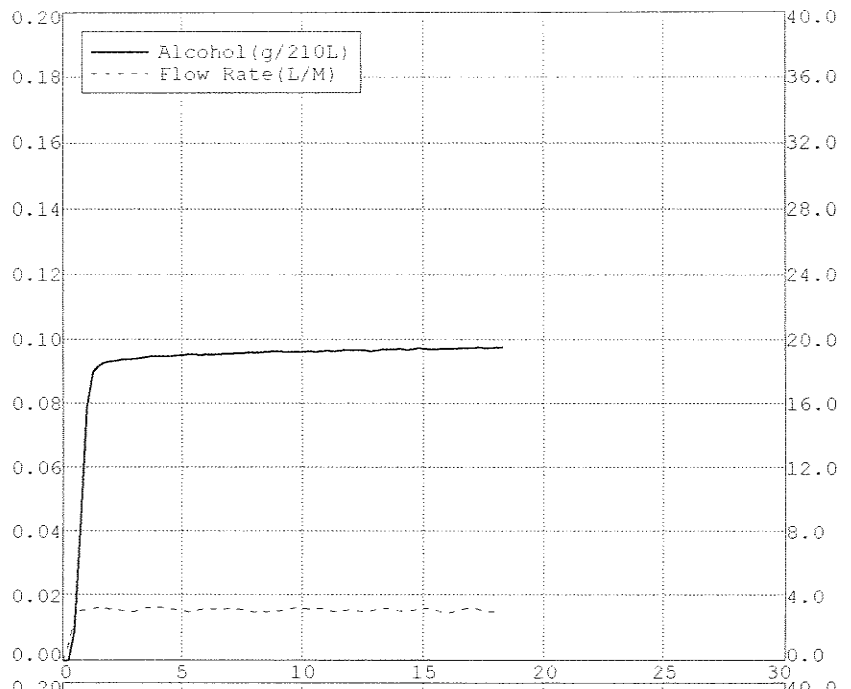

Charles B. Geisler