

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 05/27/2020

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 20040

Nominal = 0.10 g/210L

BLANK TEST	0.00	09:48
INTERNAL STANDARD	VERIFIED	09:48
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:48
BLANK TEST	0.00	09:49
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:49
BLANK TEST	0.00	09:50
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	09:51
BLANK TEST	0.00	09:51

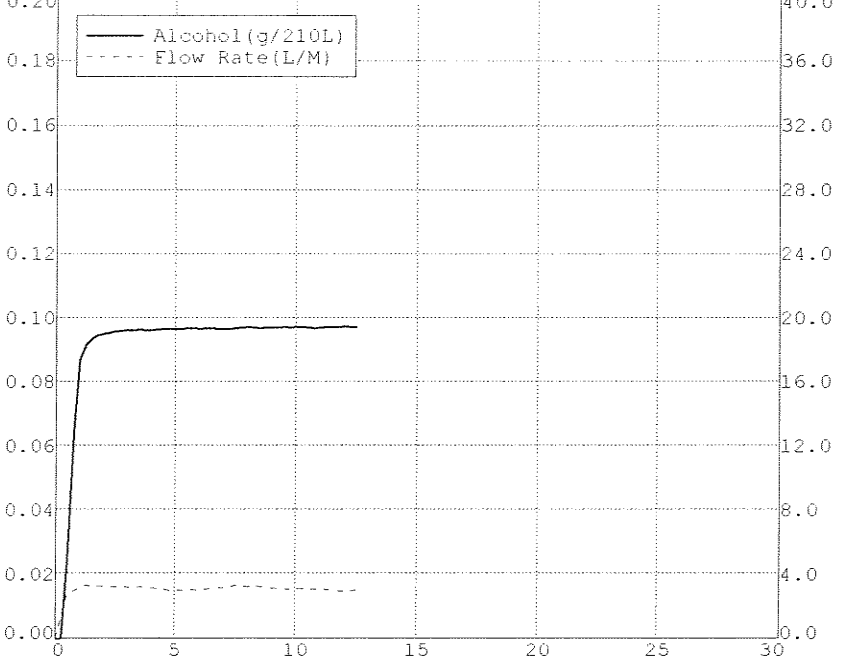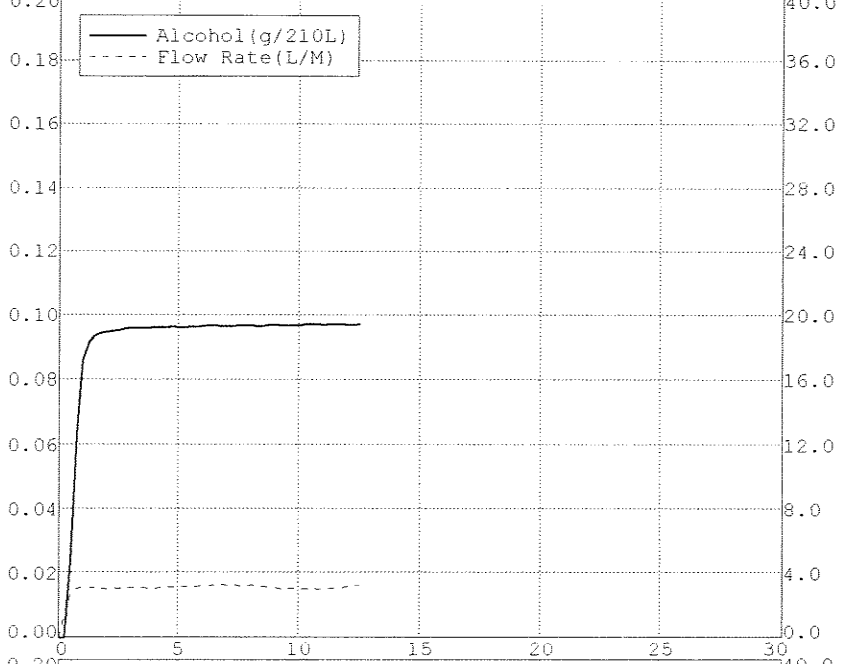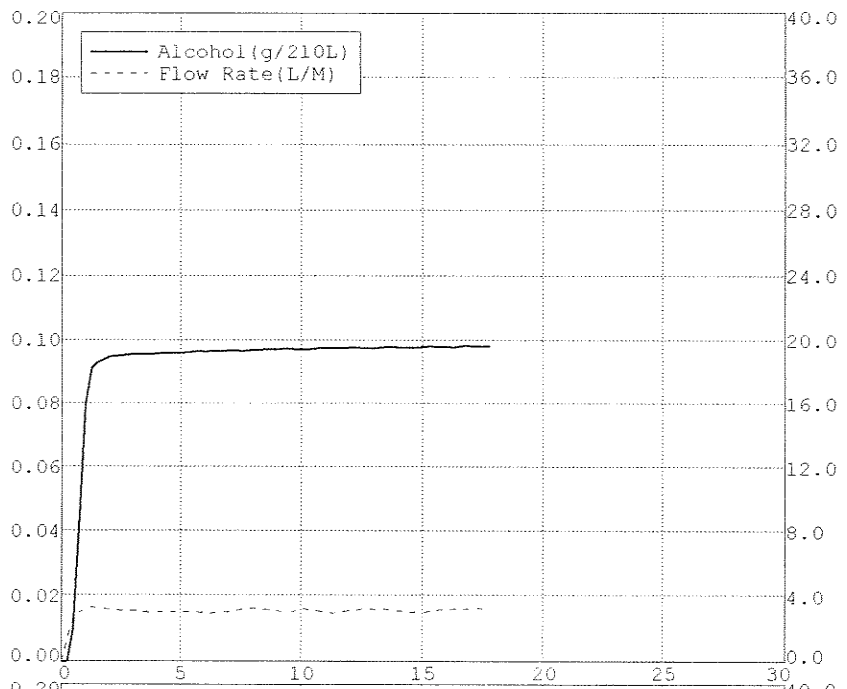

*Charles B. Geisler*