

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 06/21/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:03
INTERNAL STANDARD	VERIFIED	18:03
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:03
BLANK TEST	0.00	18:04
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:05
BLANK TEST	0.00	18:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:06
BLANK TEST	0.00	18:07

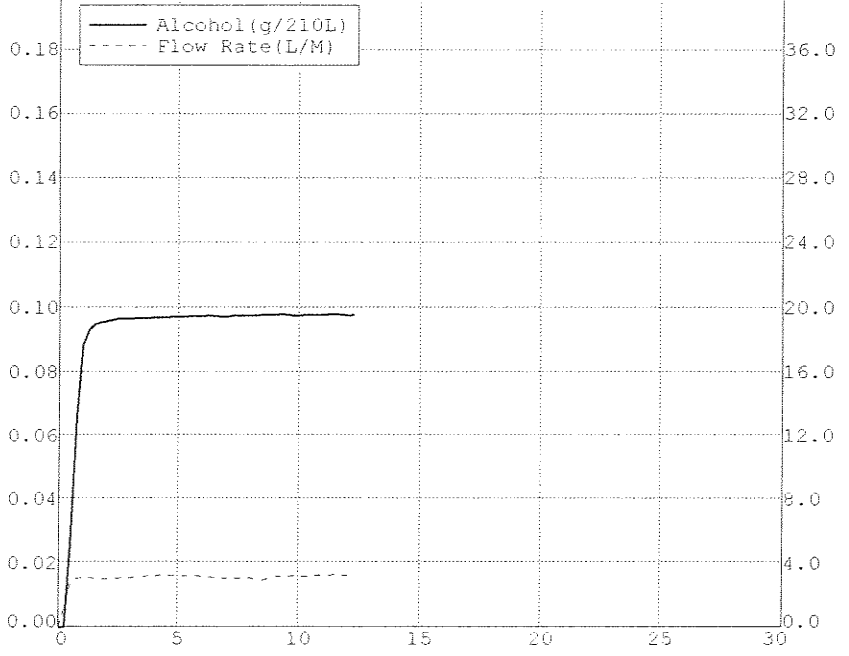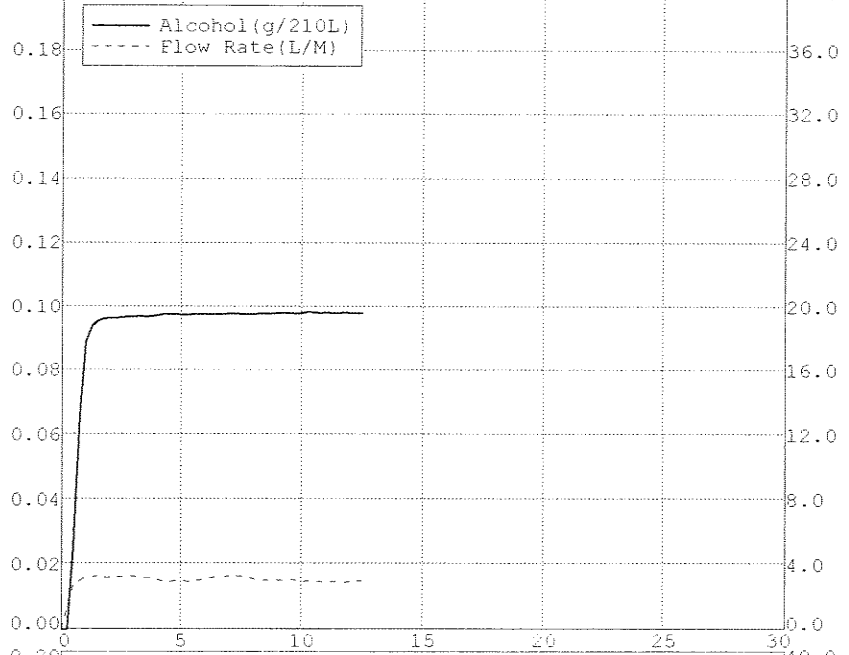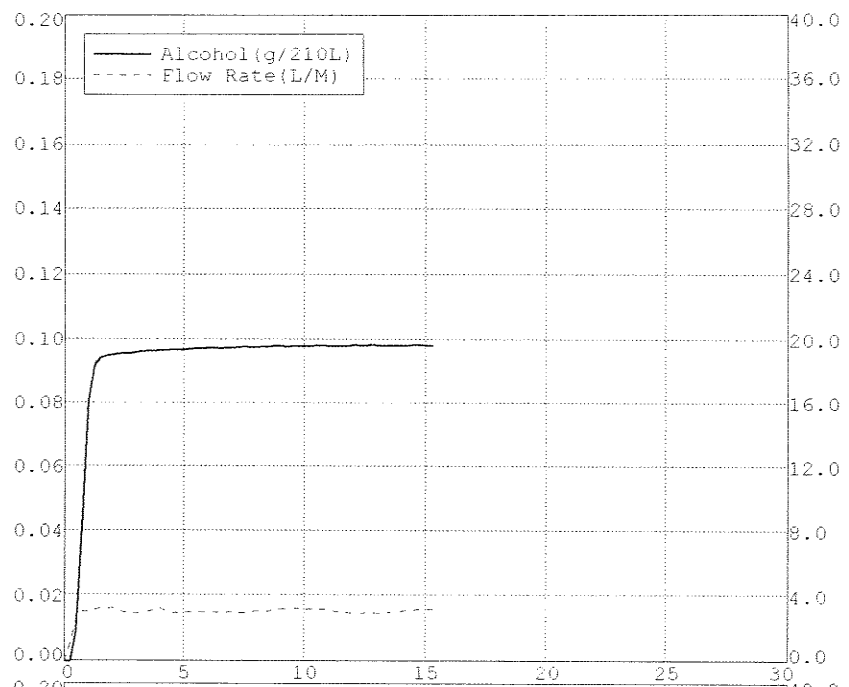

Sgt. C. B. Geisler