

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 06/29/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:42
INTERNAL STANDARD	VERIFIED	10:42
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:42
BLANK TEST	0.00	10:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:43
BLANK TEST	0.00	10:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	10:44
BLANK TEST	0.00	10:45

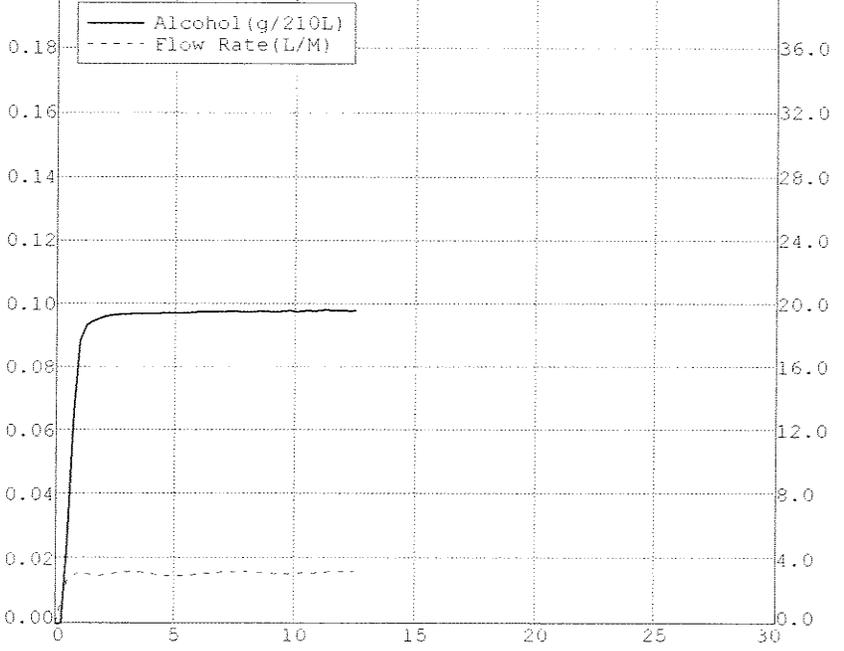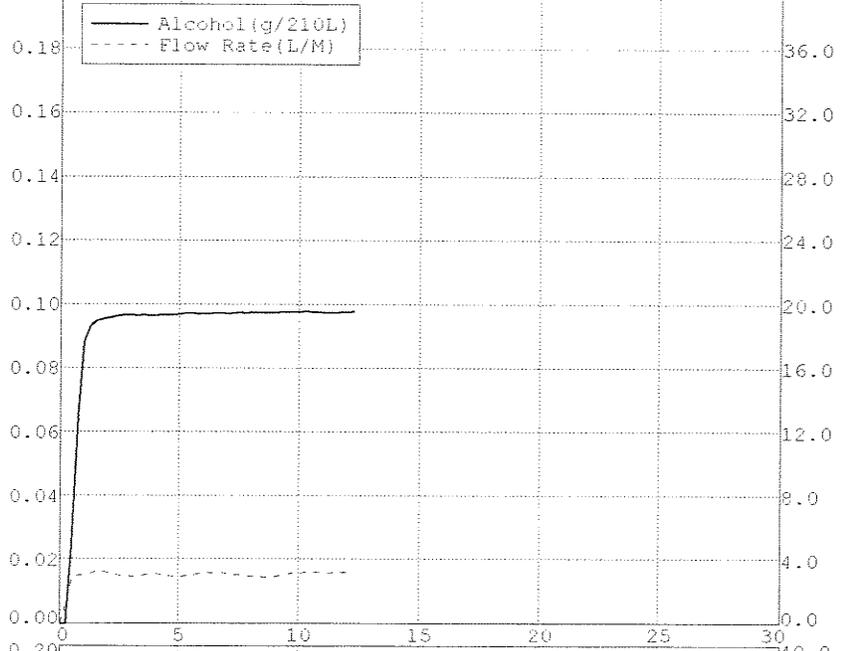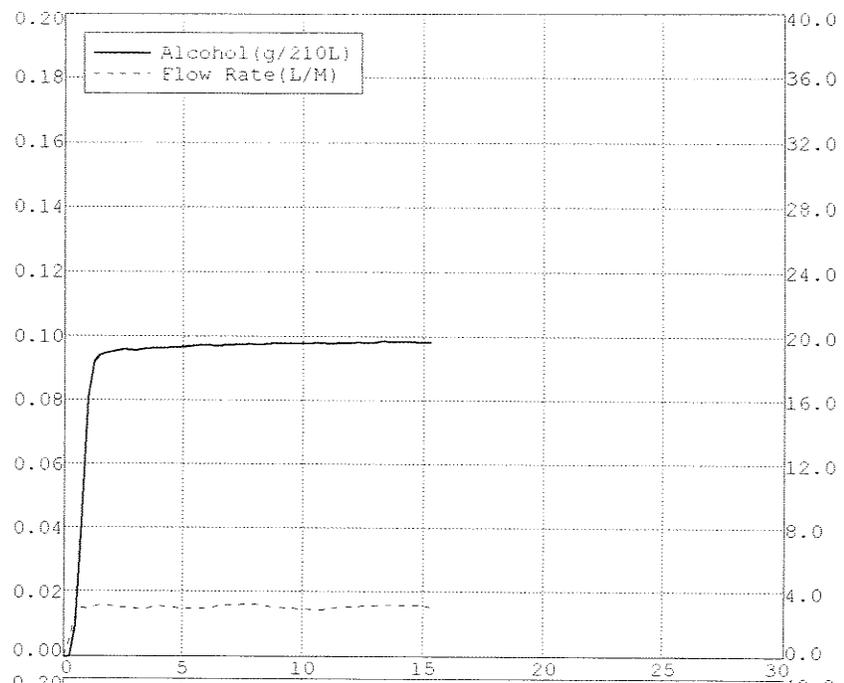

Charles B. Geisler