

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 07/03/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:04
INTERNAL STANDARD	VERIFIED	17:04
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	17:05
BLANK TEST	0.00	17:06
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	17:06
BLANK TEST	0.00	17:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	17:07
BLANK TEST	0.00	17:08

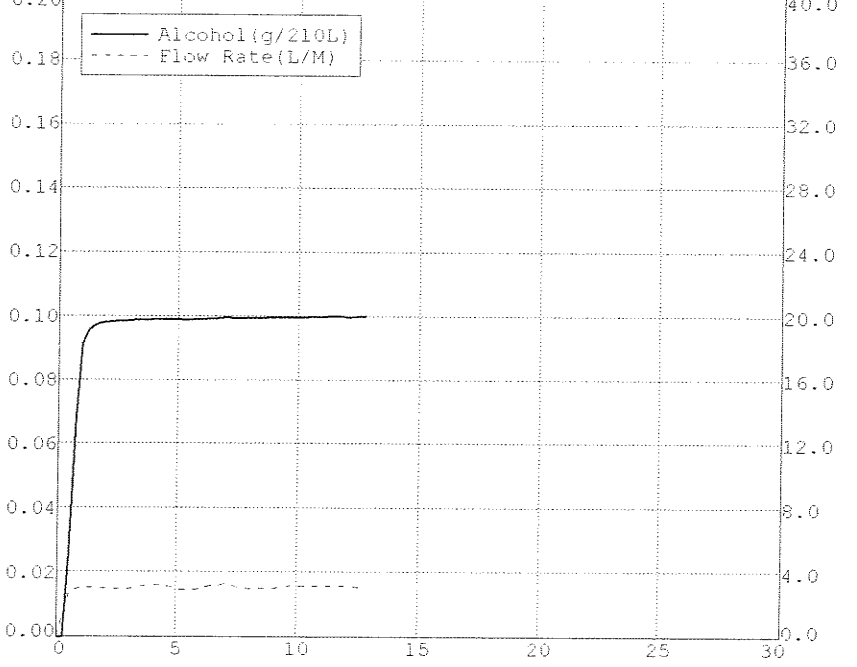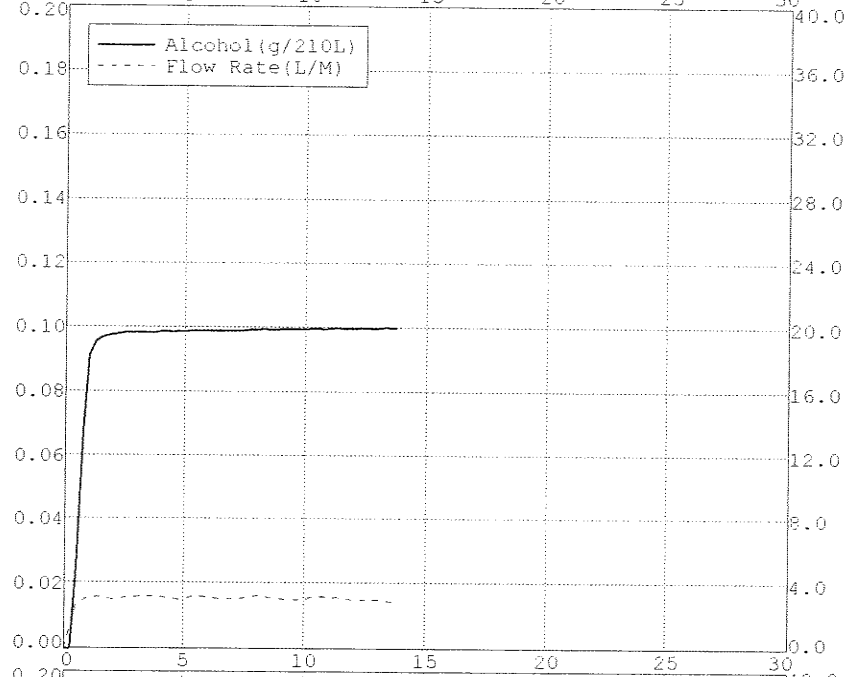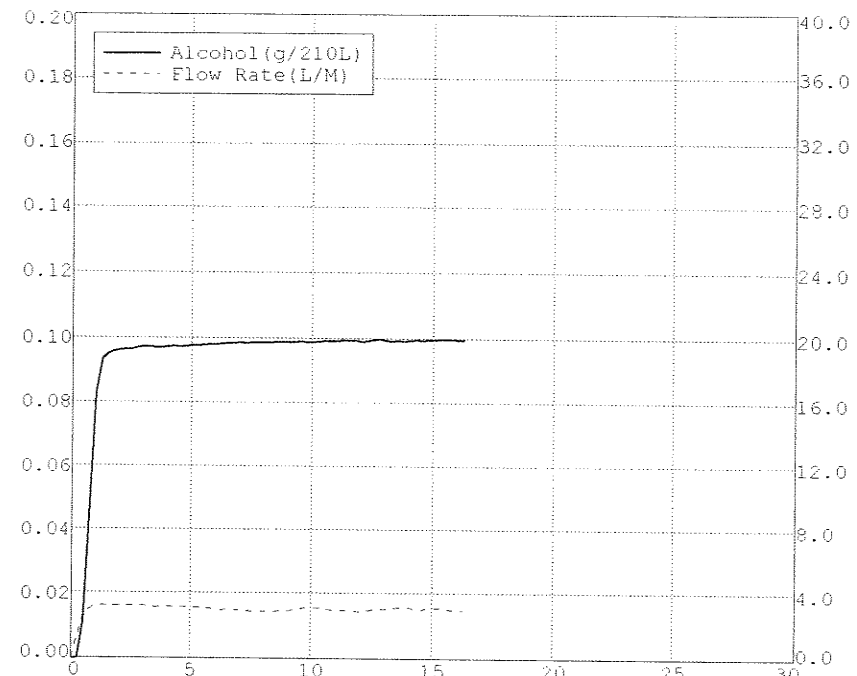

Handwritten signature: C.B. Geisler #248