

SOLUTION CHANGE




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 07/07/2020

OPERATOR NAME:  
TYLER J MORSE  
Permit #: 41959  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 20170

Nominal = 0.10 g/210L

|                         |          |       |
|-------------------------|----------|-------|
| BLANK TEST              | 0.00     | 17:57 |
| INTERNAL STANDARD       | VERIFIED | 17:57 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.10     | 17:57 |
| BLANK TEST              | 0.00     | 17:58 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.10     | 17:58 |
| BLANK TEST              | 0.00     | 17:59 |
| REFERENCE STANDARD TEMP | 34.01c   |       |
| REFERENCE STANDARD      | 0.10     | 18:00 |
| BLANK TEST              | 0.00     | 18:00 |

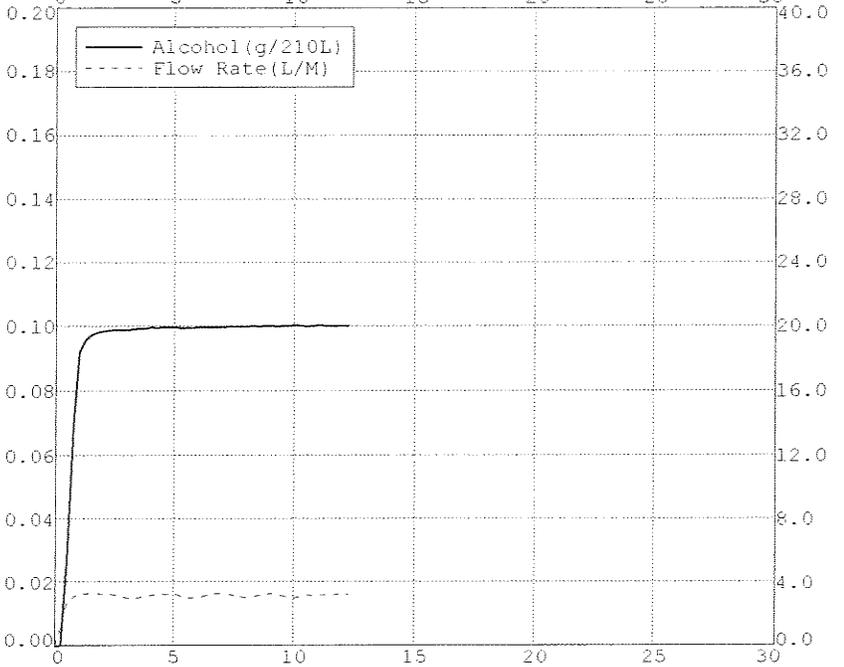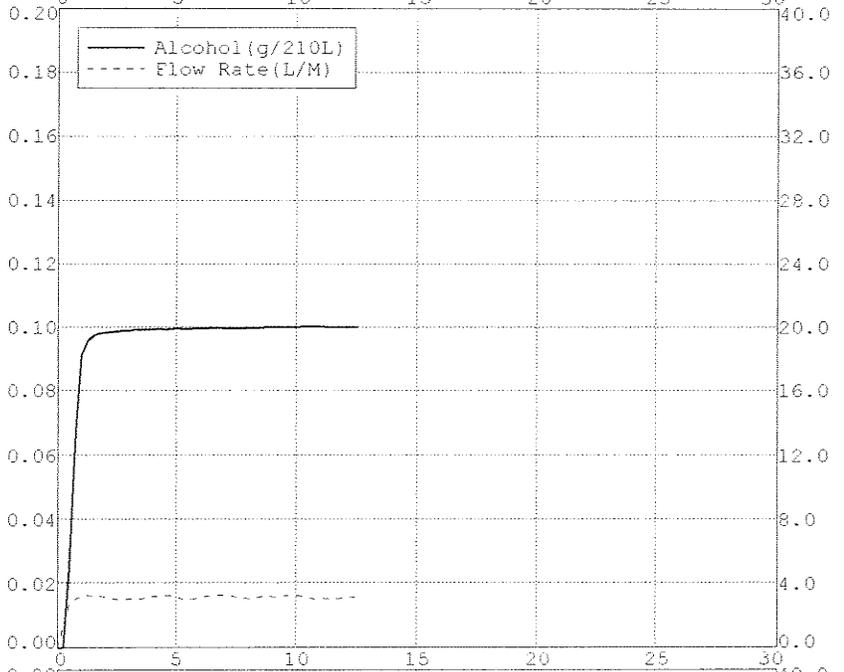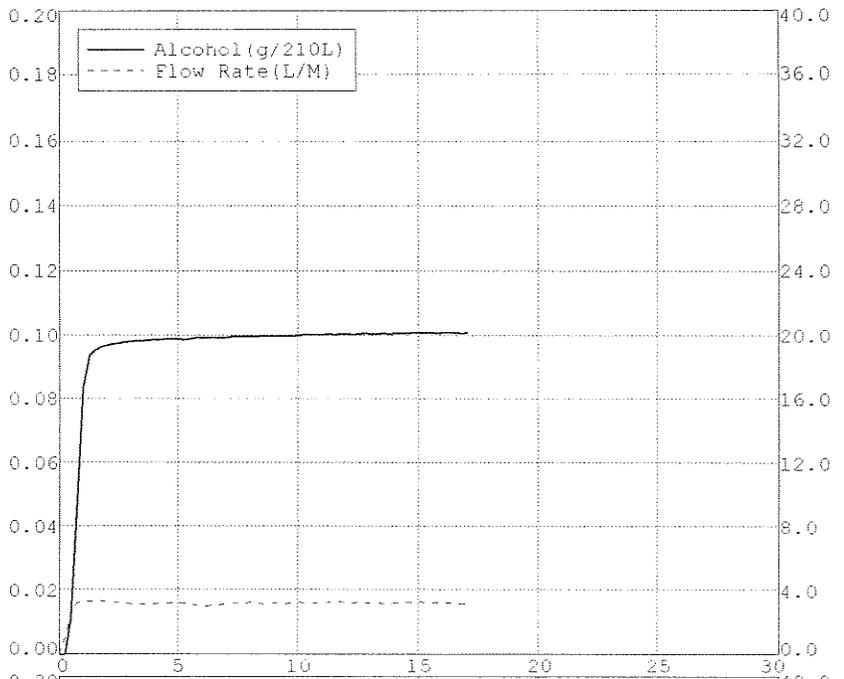

Pa #447

TJ Morse