

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 07/22/2020

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 20170

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:44
INTERNAL STANDARD	VERIFIED	17:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	17:45
BLANK TEST	0.00	17:46
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	17:46
BLANK TEST	0.00	17:47
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	17:47
BLANK TEST	0.00	17:48

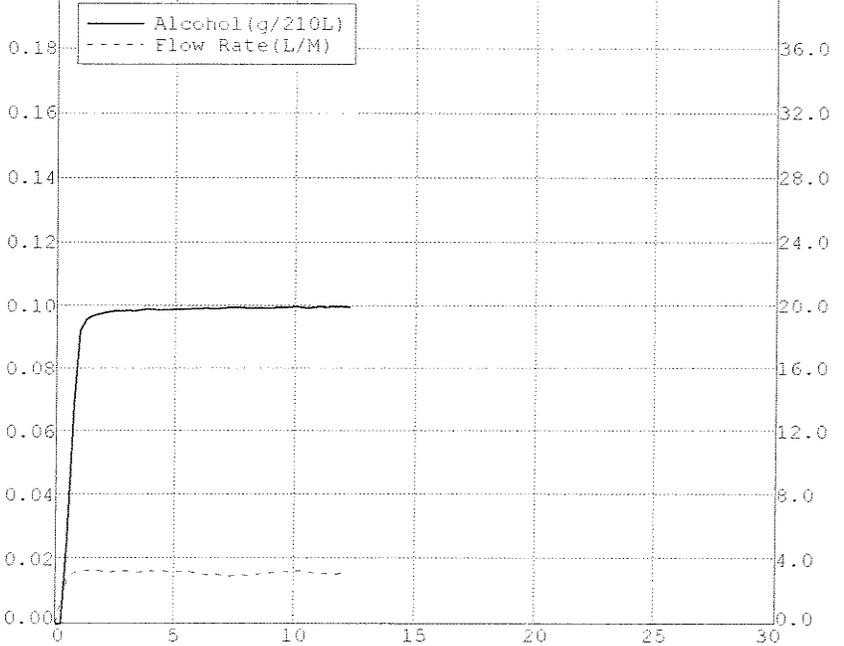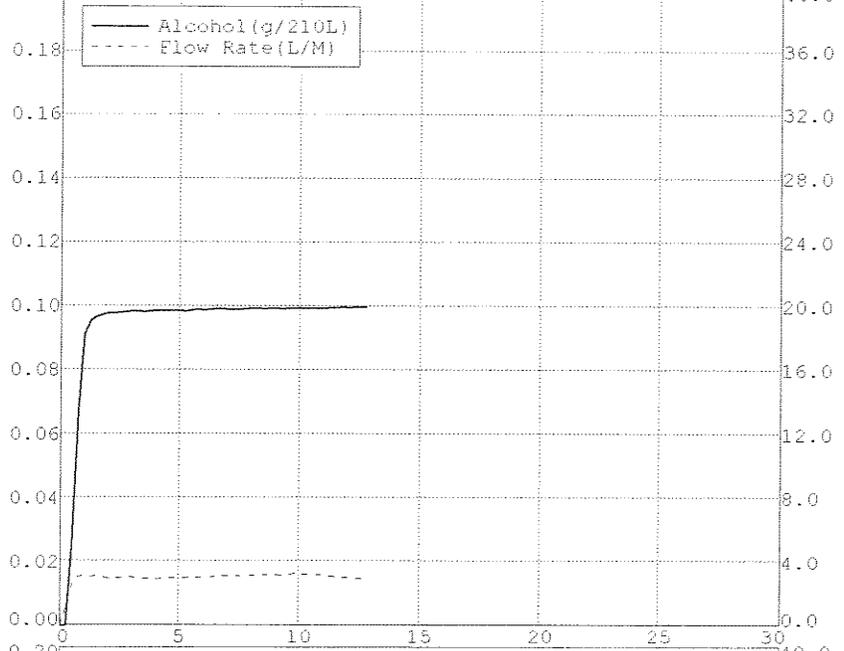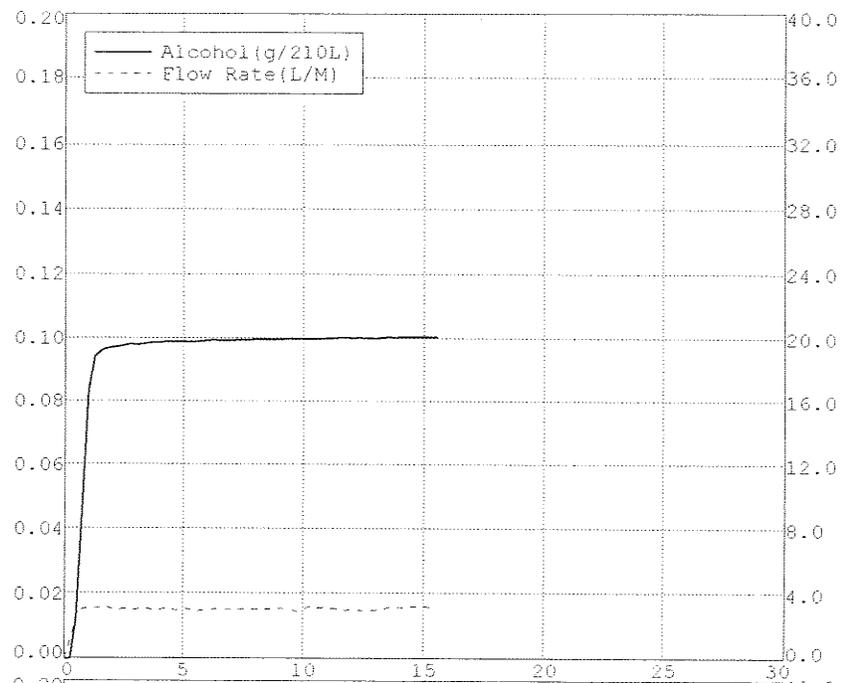

*Sgt. Chd B. [Signature] #248*