

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 08/14/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:29
INTERNAL STANDARD	VERIFIED	14:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.10	14:29
BLANK TEST	0.00	14:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:31
BLANK TEST	0.00	14:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	14:32
BLANK TEST	0.00	14:33

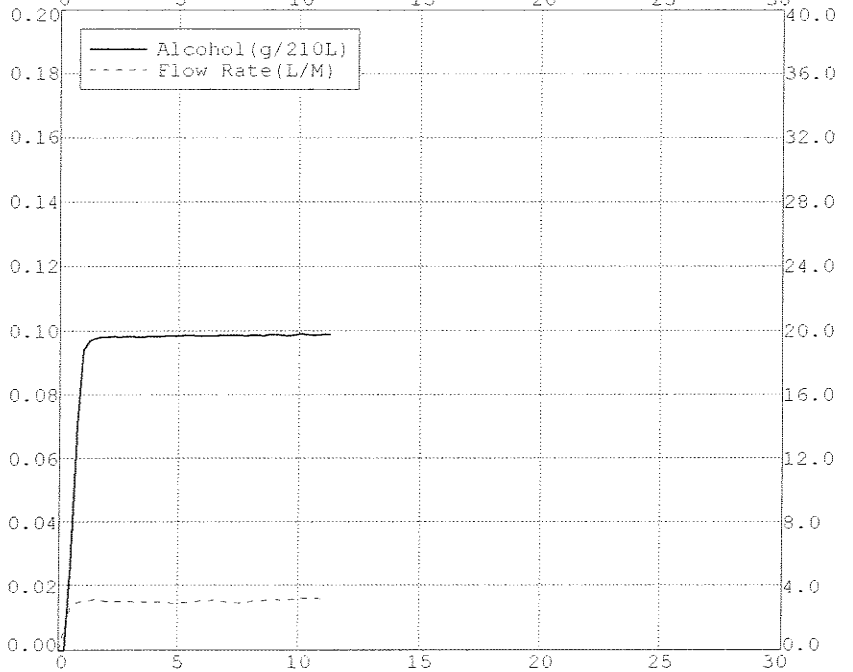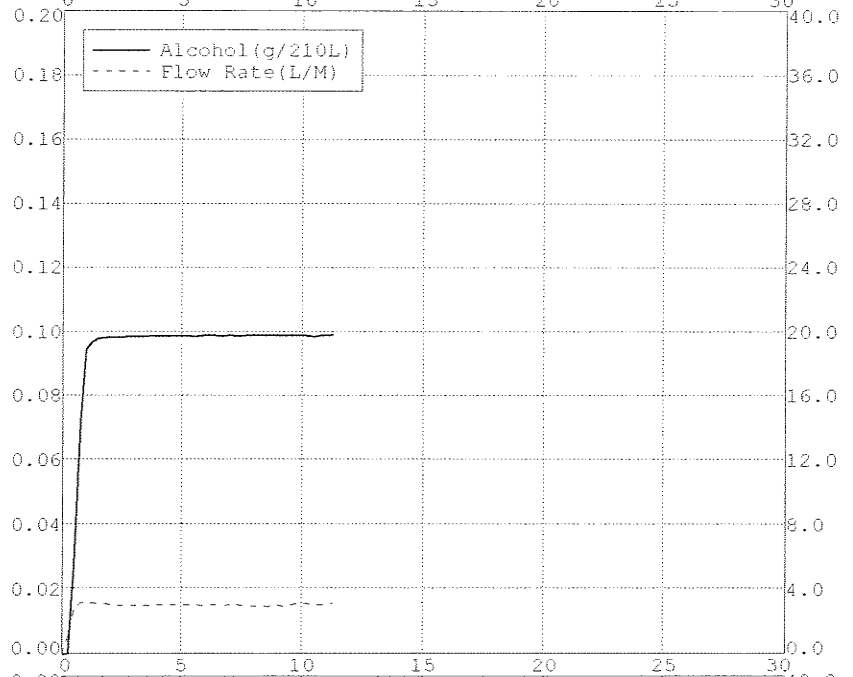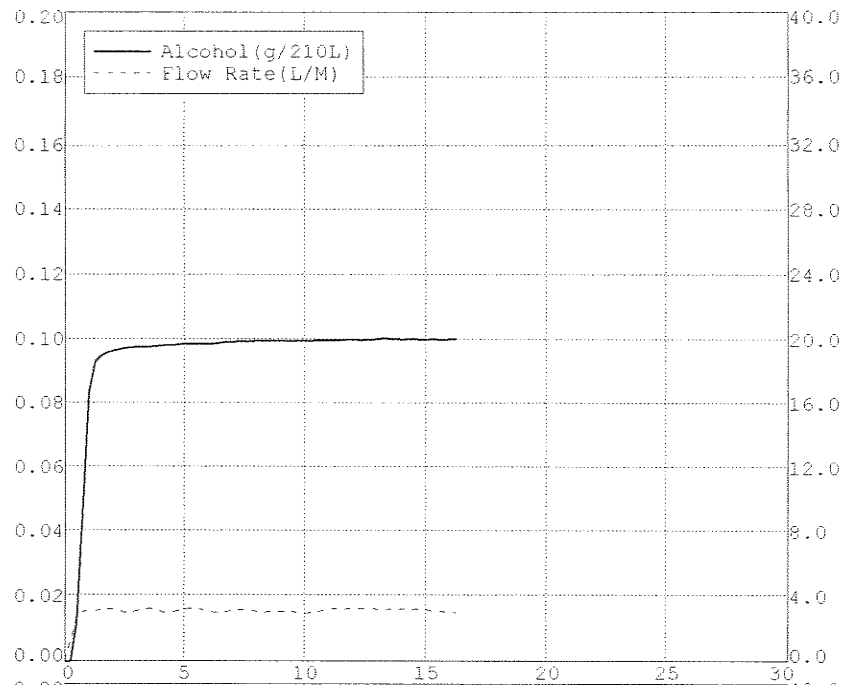

Sgt. Charles B. Geisler