

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 08/20/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	15:51
INTERNAL STANDARD	VERIFIED	15:51
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	15:51
BLANK TEST	0.00	15:52
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	15:52
BLANK TEST	0.00	15:53
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	15:53
BLANK TEST	0.00	15:54

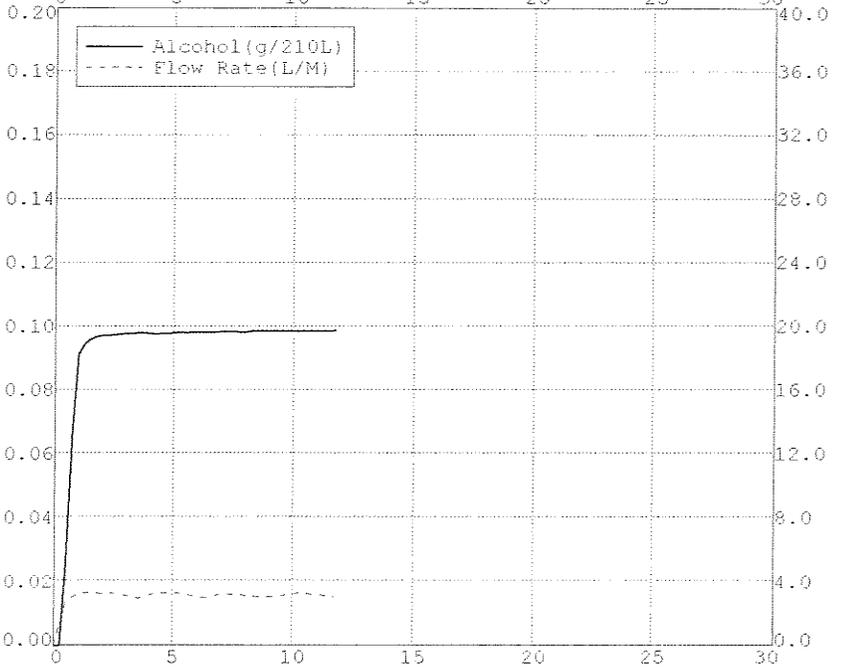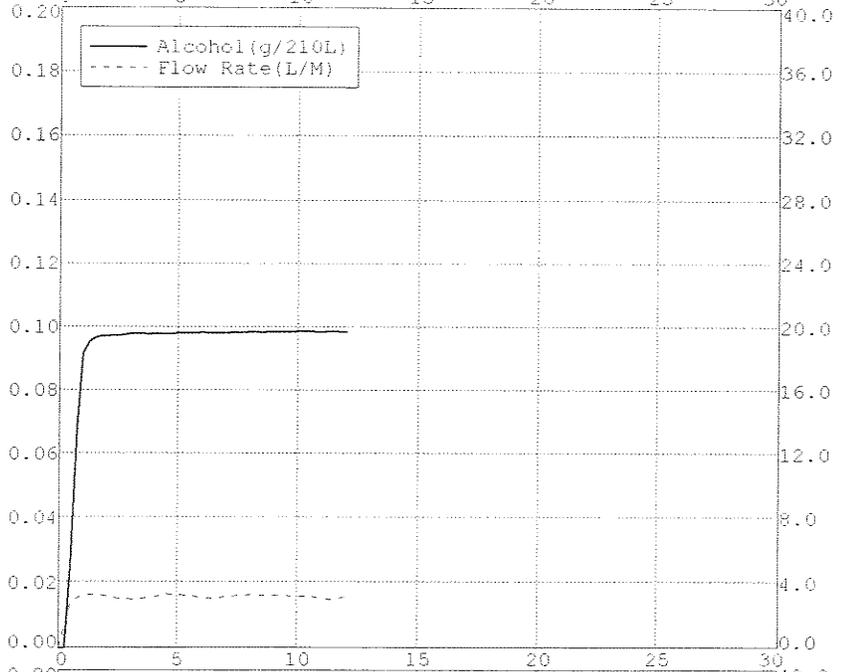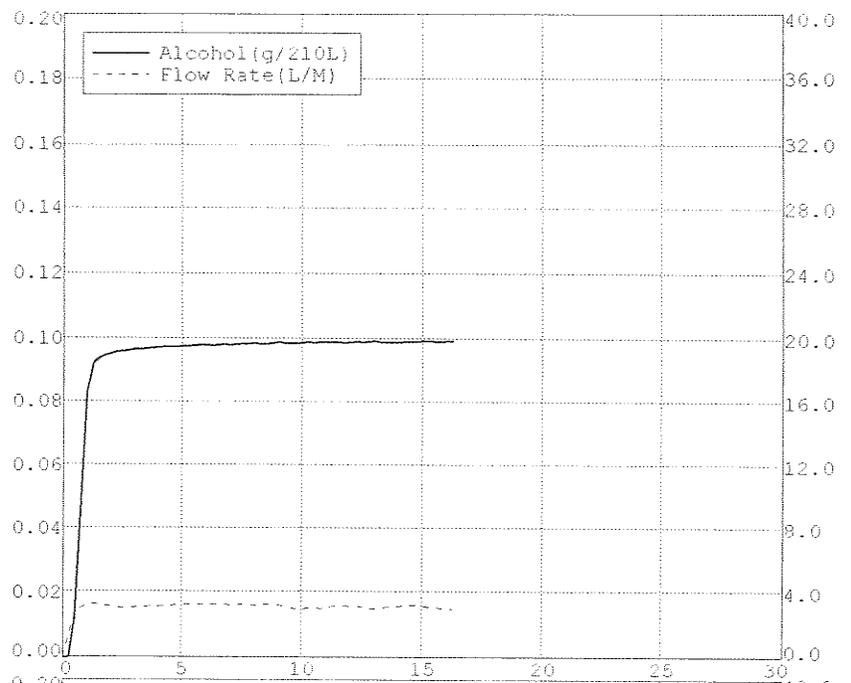

Sgt. C.B. Geisler