

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 09/02/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:09
INTERNAL STANDARD	VERIFIED	18:09
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	18:09
BLANK TEST	0.00	18:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:10
BLANK TEST	0.00	18:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:12
BLANK TEST	0.00	18:12

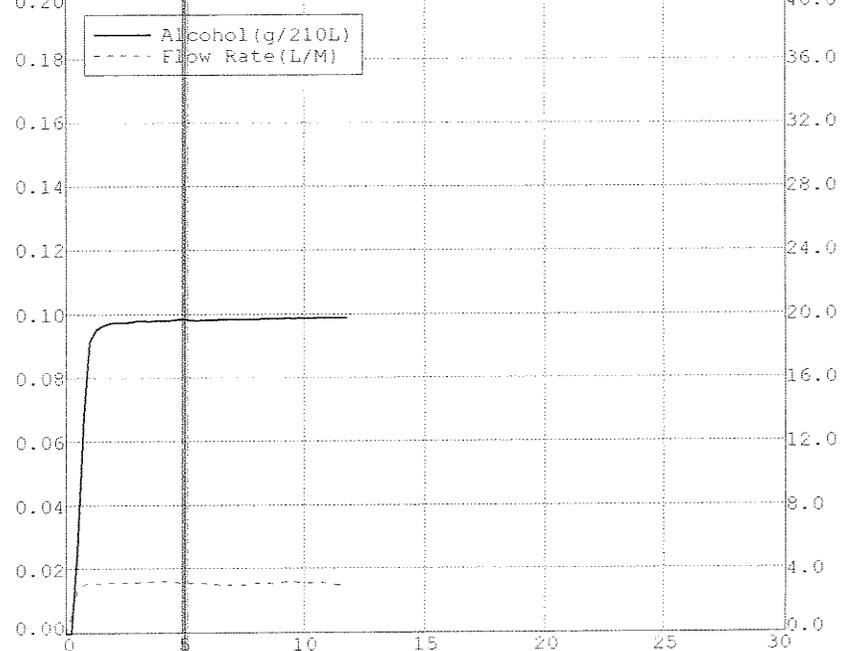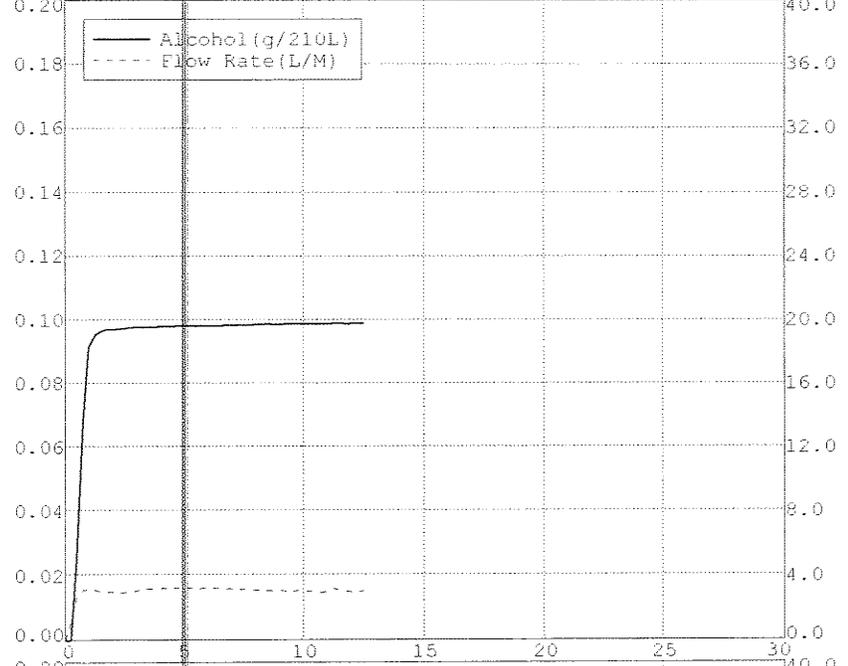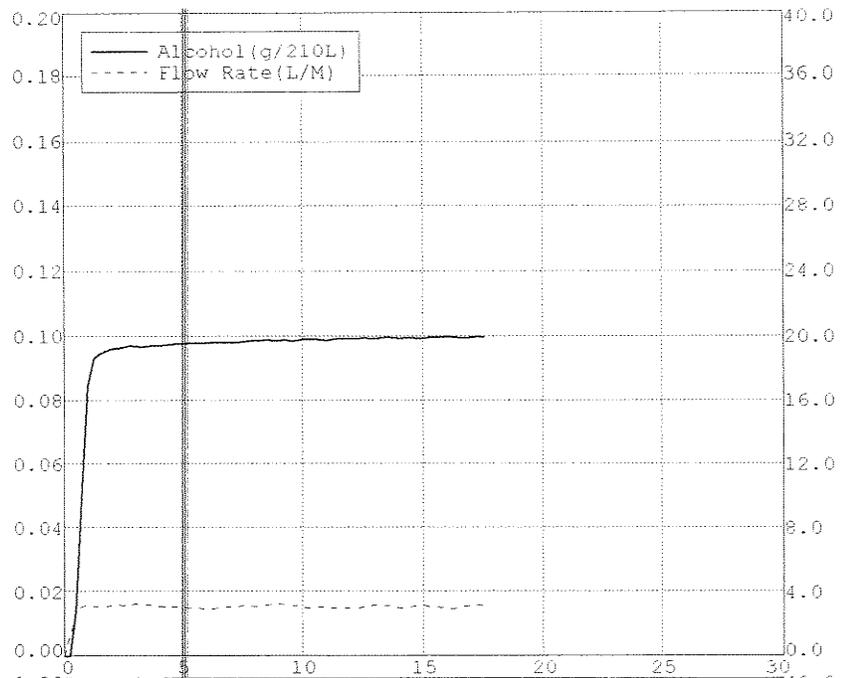

Charles B Geisler
#240