

SUPERVISOR TEST




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 09/25/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20240

Nominal = 0.10 g/210L

BLANK TEST	0.00	18:14
INTERNAL STANDARD	VERIFIED	18:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.10	18:15
BLANK TEST	0.00	18:16
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	18:16
BLANK TEST	0.00	18:17
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.09	18:17
BLANK TEST	0.00	18:18

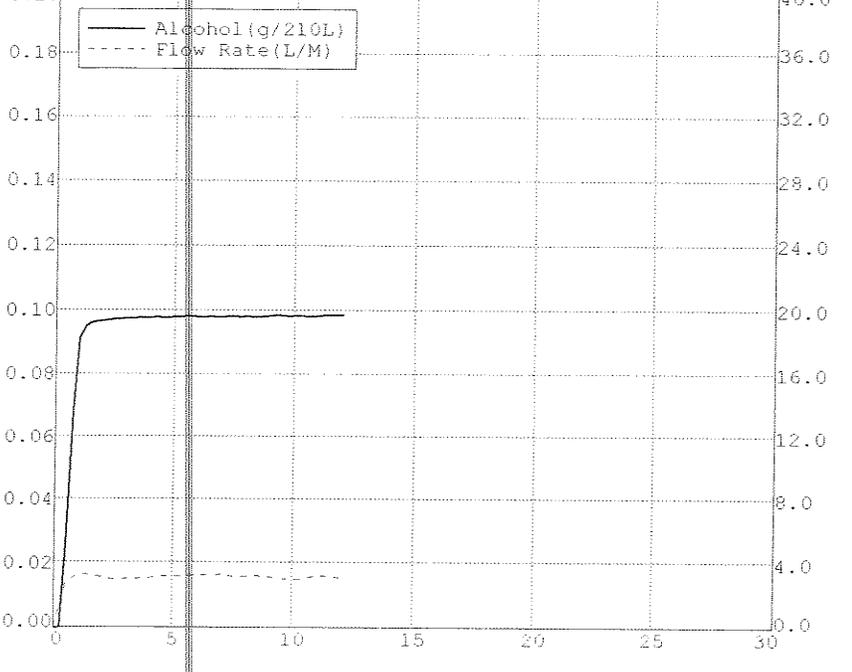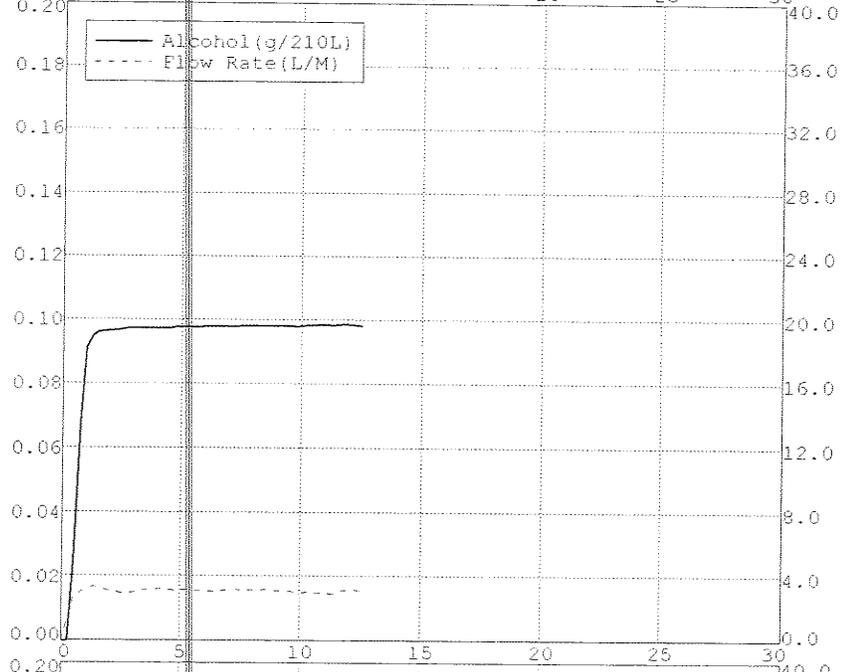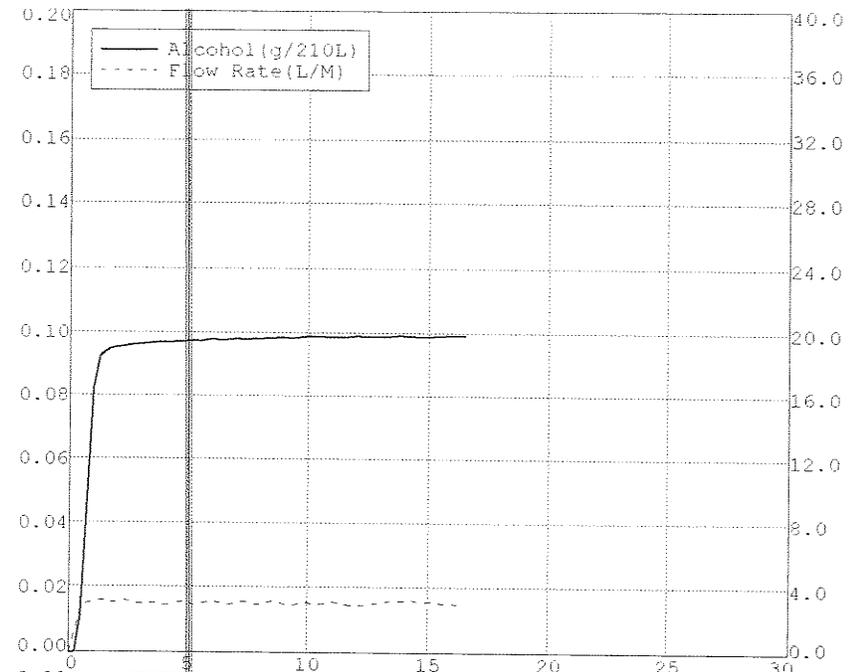

Sgt. Charles B. Geisler