

SOLUTION CHANGE




WARREN CO.
SHERIFF'S OFFICE
DATAMASTER dmt: 106606

Date: 10/01/2020

OPERATOR NAME:
CHARLES B GEISLER
Permit #: 33757
Operator Agency/Dept: WARREN CO. SO
Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:47
INTERNAL STANDARD	VERIFIED	17:47
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:47
BLANK TEST	0.00	17:48
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:48
BLANK TEST	0.00	17:49
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:50
BLANK TEST	0.00	17:50

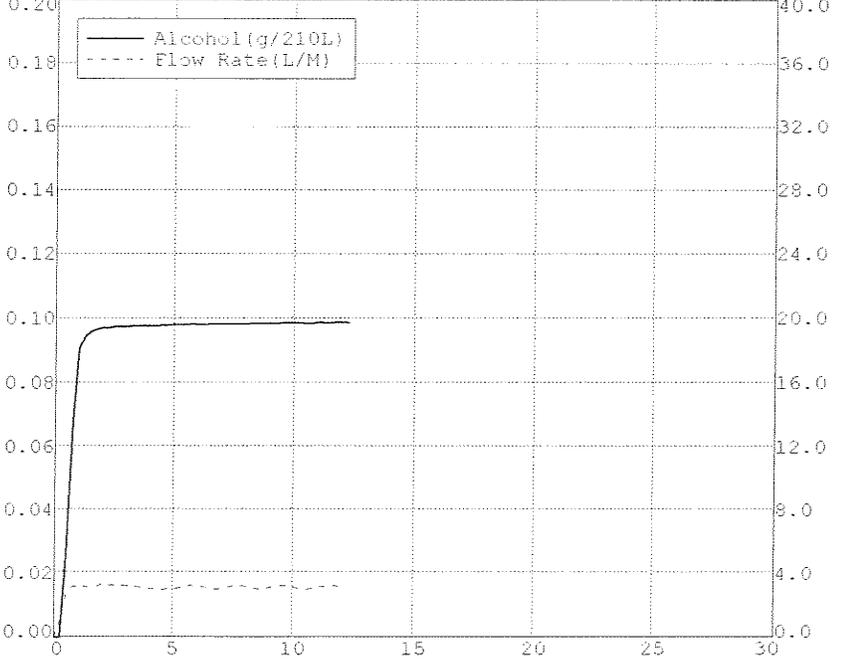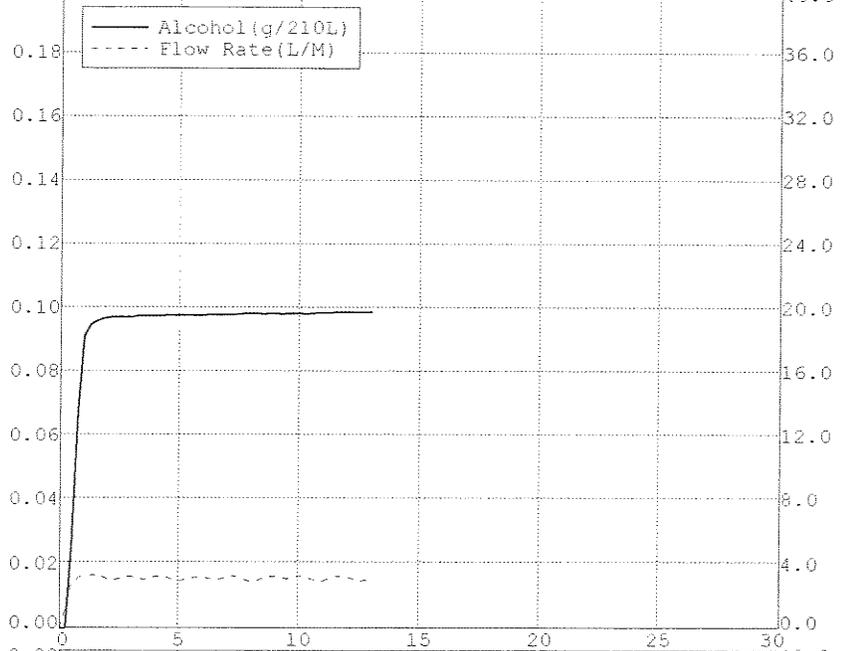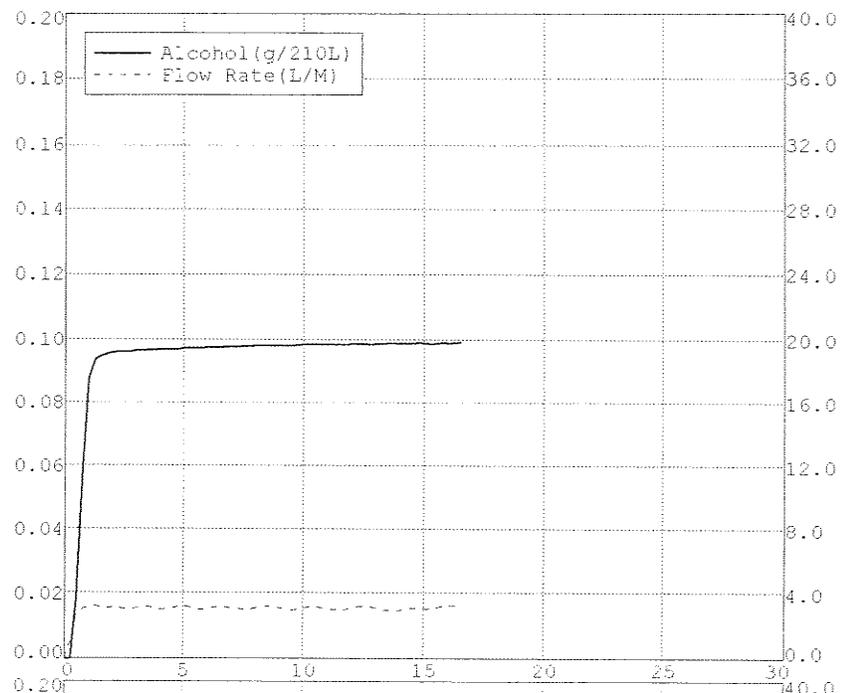

Handwritten signatures and initials:
J. Bl... B... #24