

SUPERVISOR TEST




WARREN CO.  
SHERIFF'S OFFICE  
DATAMASTER dmt: 106606

Date: 10/20/2020

OPERATOR NAME:  
CHARLES B GEISLER  
Permit #: 33757  
Operator Agency/Dept: WARREN CO. SO  
Reference Standard #: 20340

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:10
INTERNAL STANDARD	VERIFIED	17:10
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:11
BLANK TEST	0.00	17:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:12
BLANK TEST	0.00	17:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.09	17:13
BLANK TEST	0.00	17:14

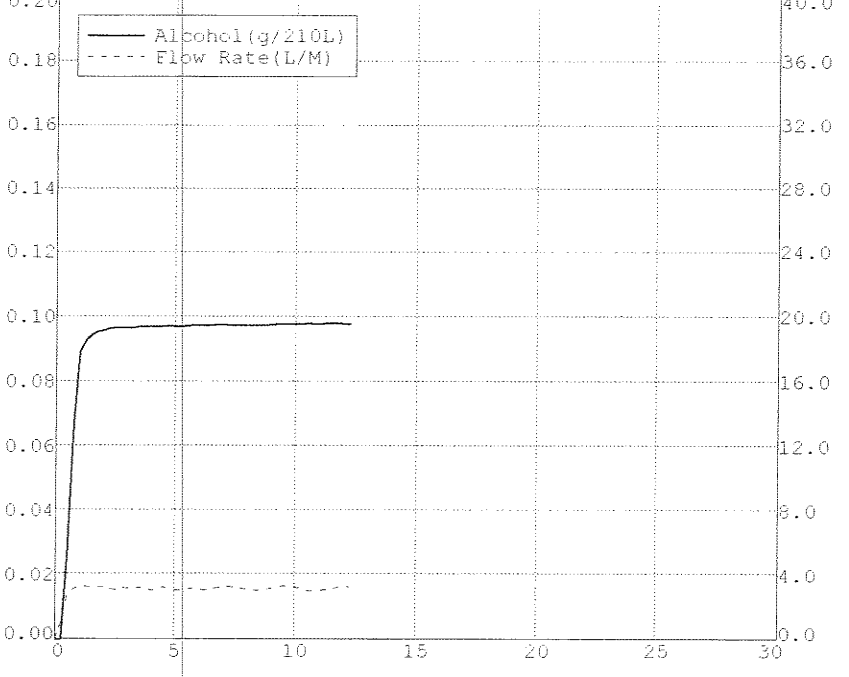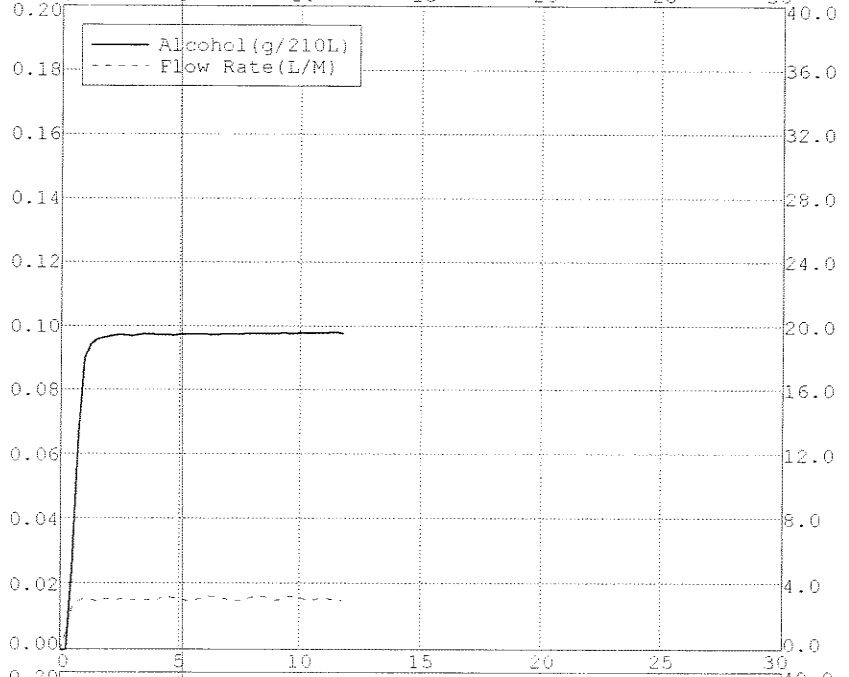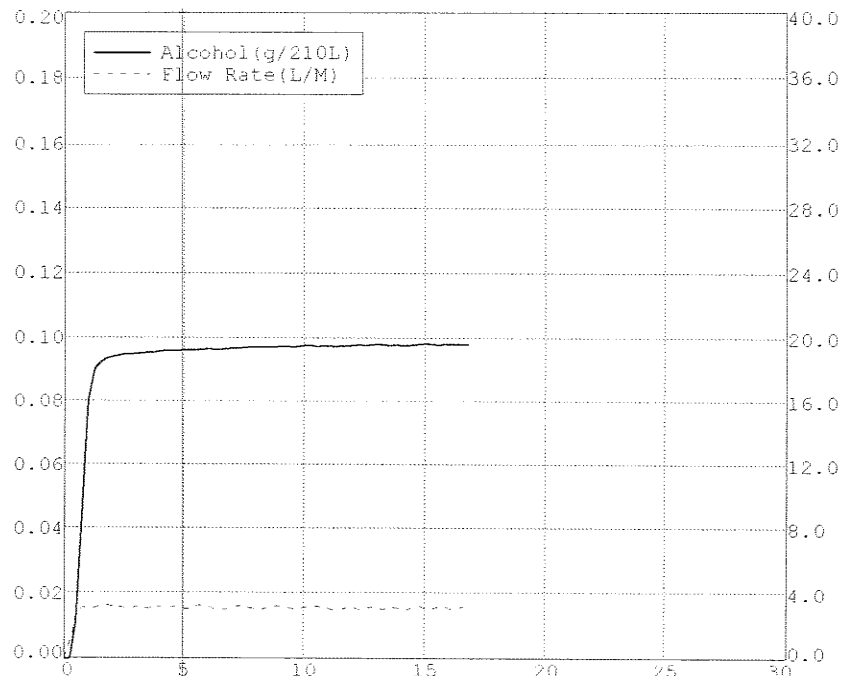

*Chl-B* *CG #241*